


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020818\
 Data File : BF102870.D
 Acq On : 8 Feb 2018 22:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

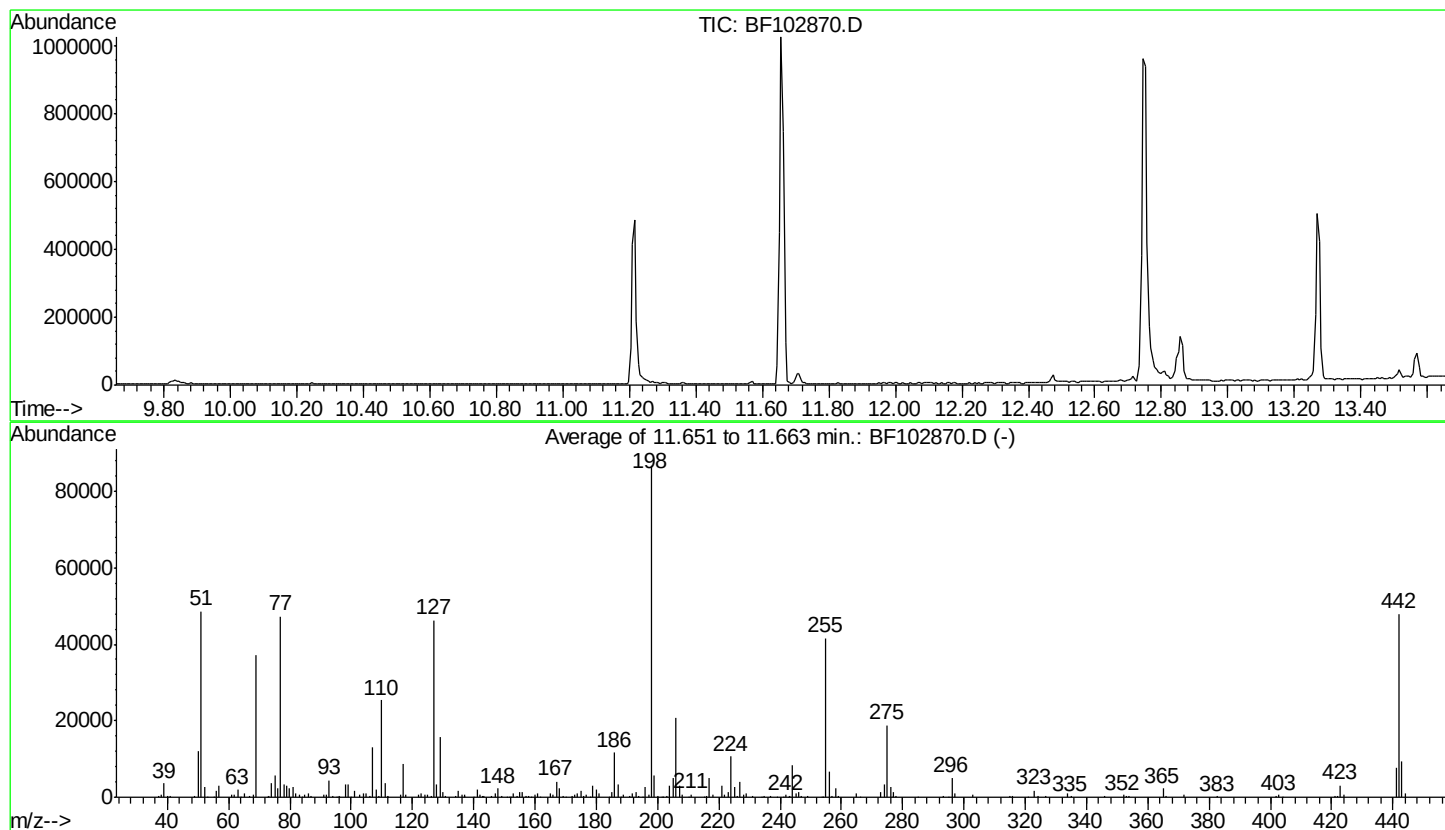

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	48685	PASS
68	69	0.00	2	1.9	691	PASS
69	198	0.00	100	43.0	37317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	46330	PASS
197	198	0.00	2	0.8	725	PASS
198	198	100	100	100.0	86704	PASS
199	198	5	9	6.5	5614	PASS
275	198	10	60	21.7	18804	PASS
365	198	1	100	2.6	2287	PASS
441	443	0.01	100	81.8	7747	PASS
442	198	50	100	55.2	47901	PASS
443	442	15	24	19.8	9471	PASS