
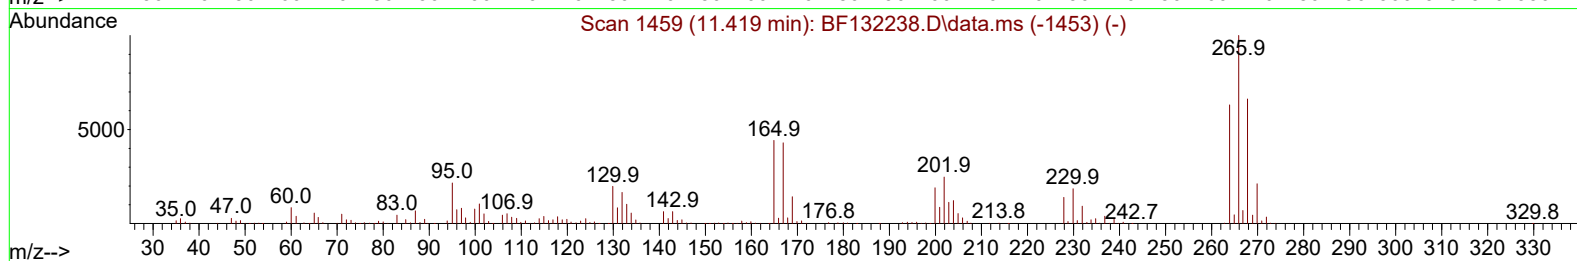
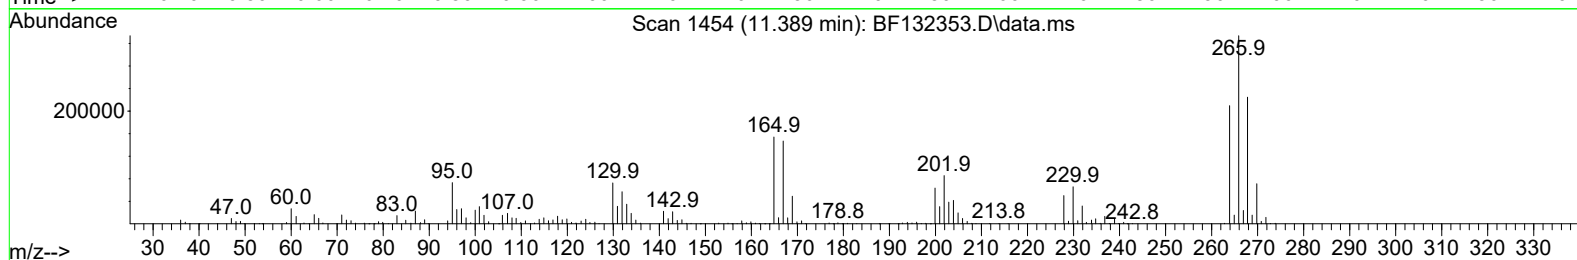


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020823\  
Data File : BF132353.D  
Acq On    : 08 Feb 2023  12:04  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Feb 09 04:06:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 01:56:26 2023
Response via : Initial Calibration

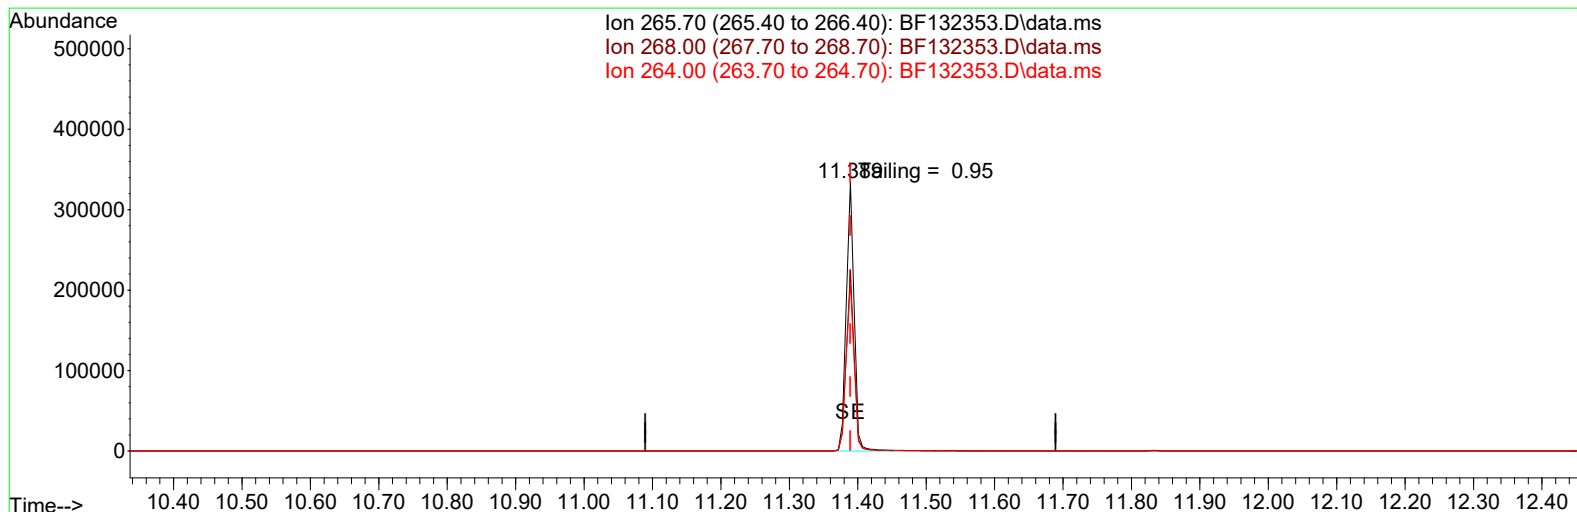

TIC: BF132353.D\data.ms

(70) Pentachlorophenol (C)




11.389min (+ 0.000) 324186.36 ng

response **270608**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	67.33
264.00	63.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020823\
Data File : BF132353.D
Acq On : 08 Feb 2023 12:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 04:06:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 01:56:26 2023
Response via : Initial Calibration

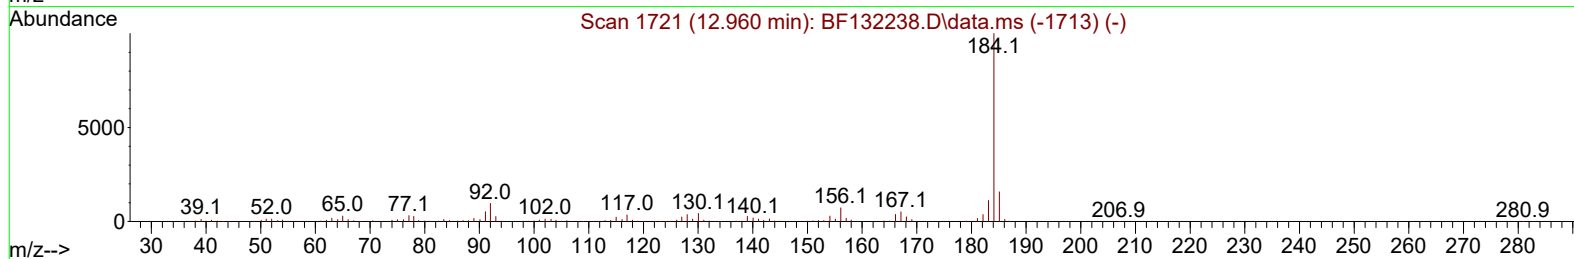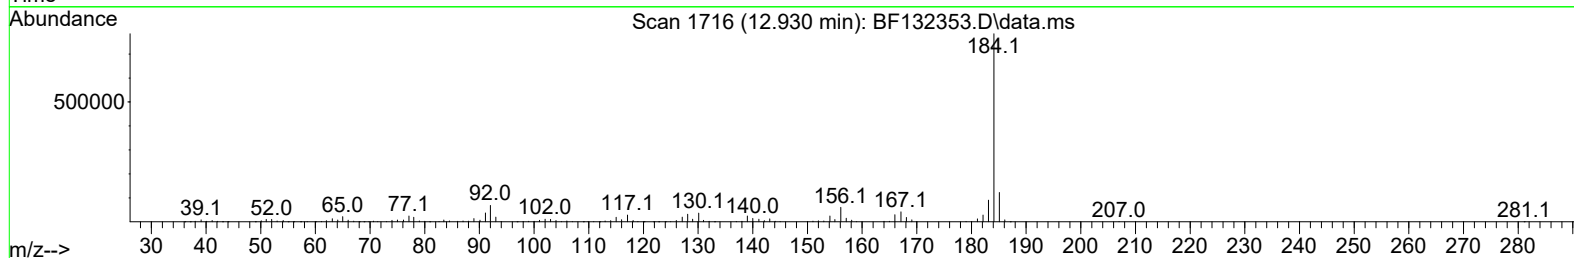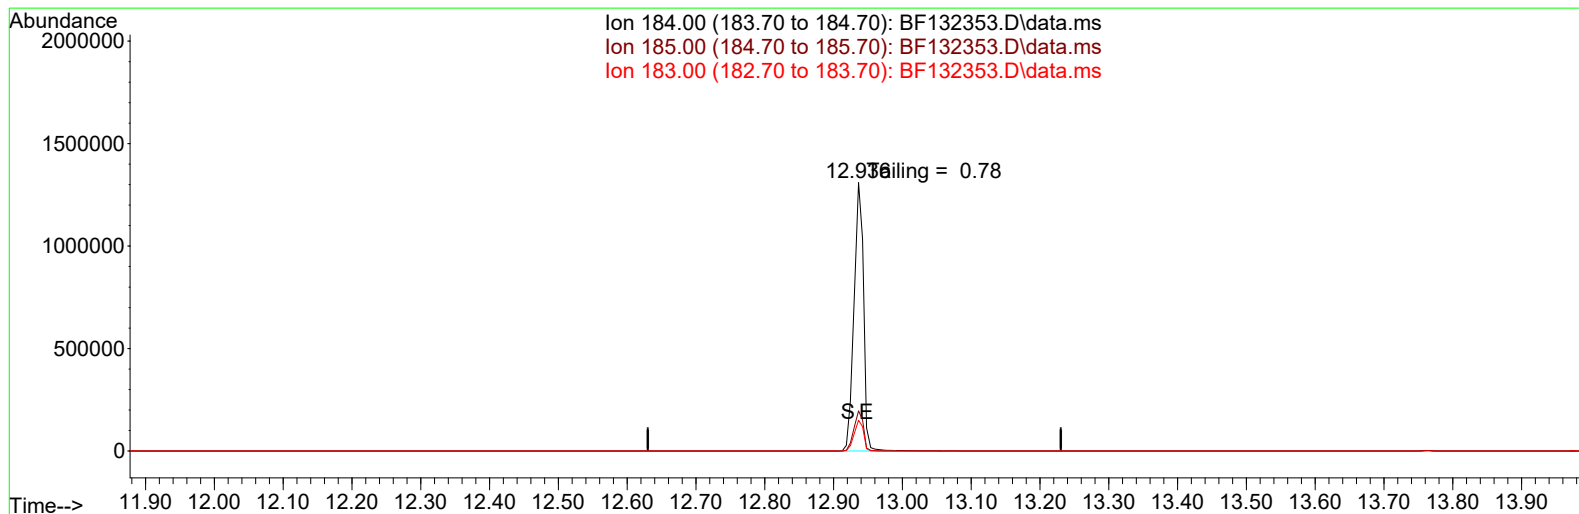

TIC: BF132353.D\data.ms

(77) Benzidine

12.930min (-12.930) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.70	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00