


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020823\
Data File : BF132353.D
Acq On : 08 Feb 2023 12:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 09 01:56:26 2023

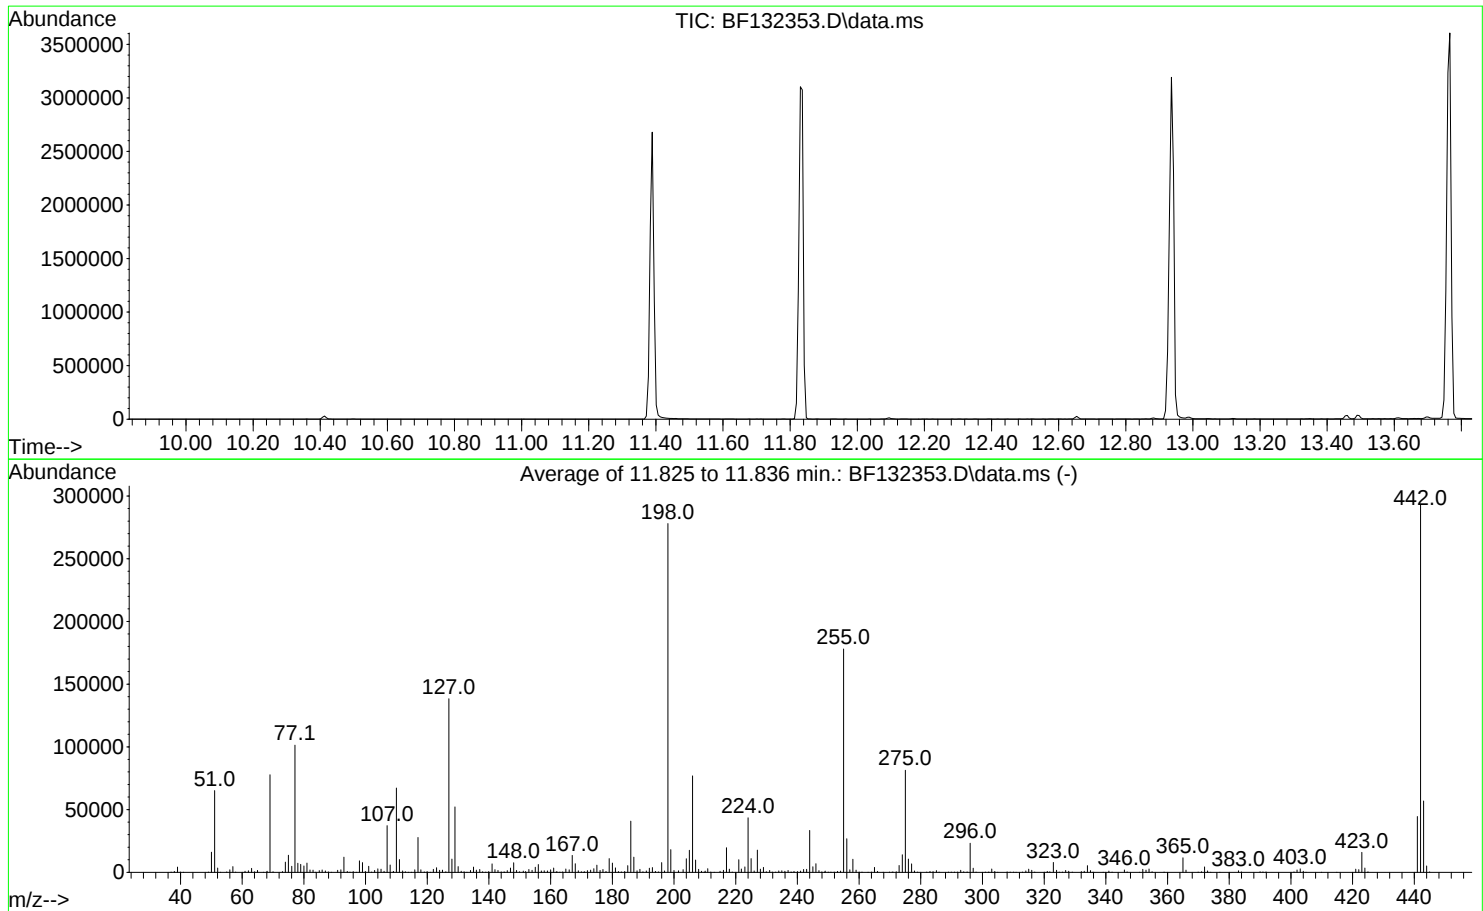




AutoFind: Scans 1528, 1529, 1530; Background Corrected with Scan 1523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	65091	PASS
68	69	0.00	2	1.1	855	PASS
69	198	0.00	100	28.0	77800	PASS
70	69	0.00	2	0.6	457	PASS
127	198	10	80	49.8	138339	PASS
197	198	0.00	2	0.4	1063	PASS
198	198	100	100	100.0	278016	PASS
199	198	5	9	6.5	18020	PASS
275	198	10	60	29.3	81389	PASS
365	198	1	100	4.1	11534	PASS
441	198	0.01	100	16.0	44527	PASS
442	442	50	100	100.0	293285	PASS
443	442	15	24	19.4	56855	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020823\
 Data File : BF132353.D
 Acq On : 08 Feb 2023 12:04
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 09 04:06:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 09 01:56:26 2023
 Response via : Initial Calibration

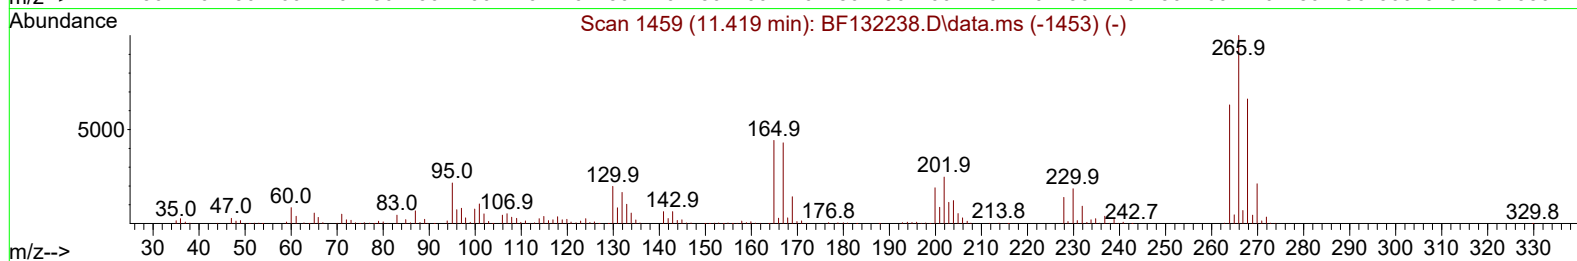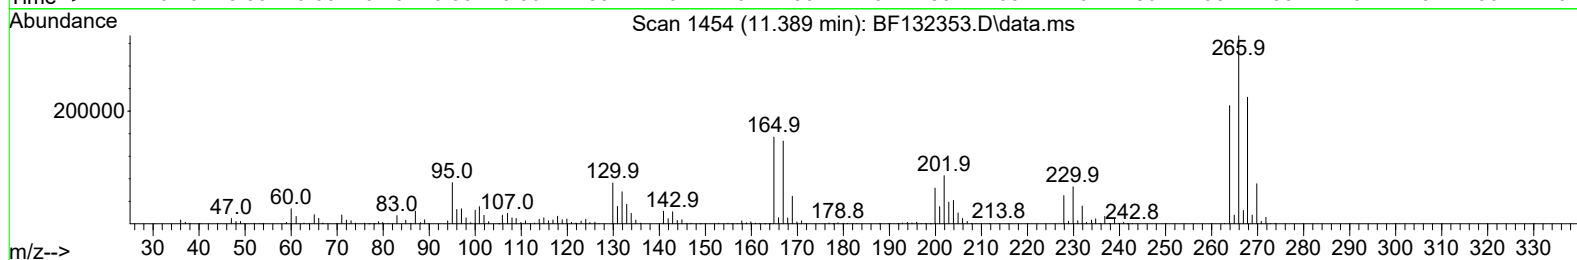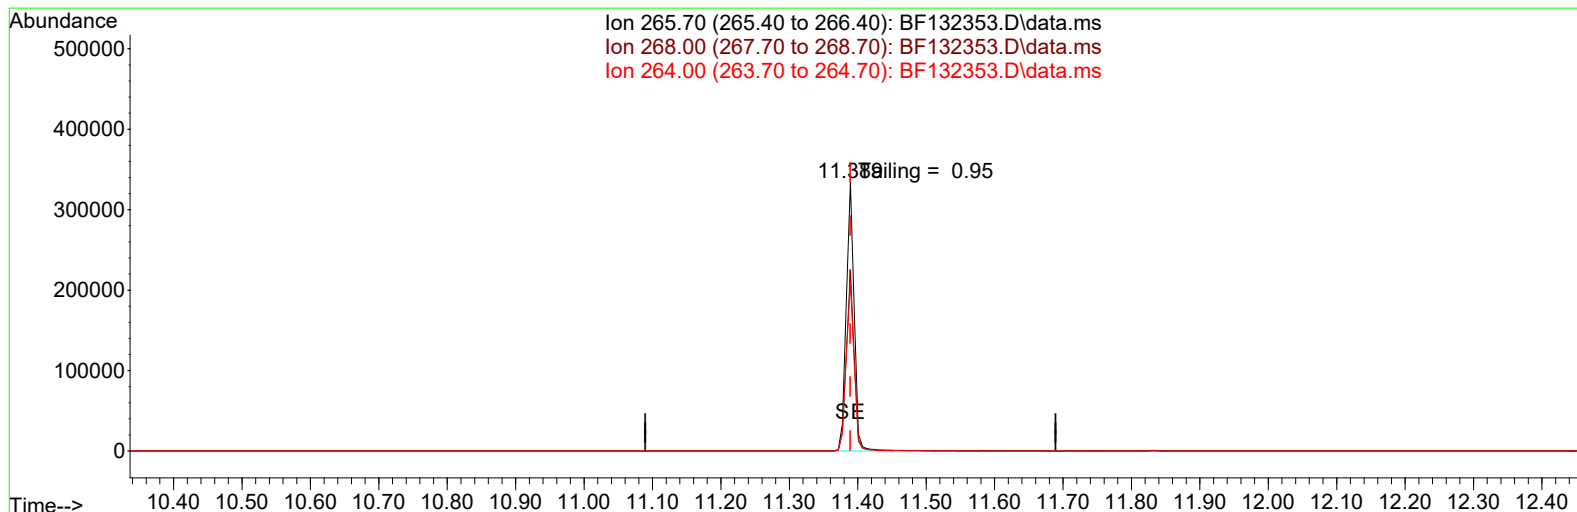

TIC: BF132353.D\data.ms

(70) Pentachlorophenol (C)

11.389min (+ 0.000) 324186.36 ng




response 270608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	67.33
264.00	63.10	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020823\
Data File : BF132353.D
Acq On : 08 Feb 2023 12:04
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 09 04:06:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 01:56:26 2023
Response via : Initial Calibration

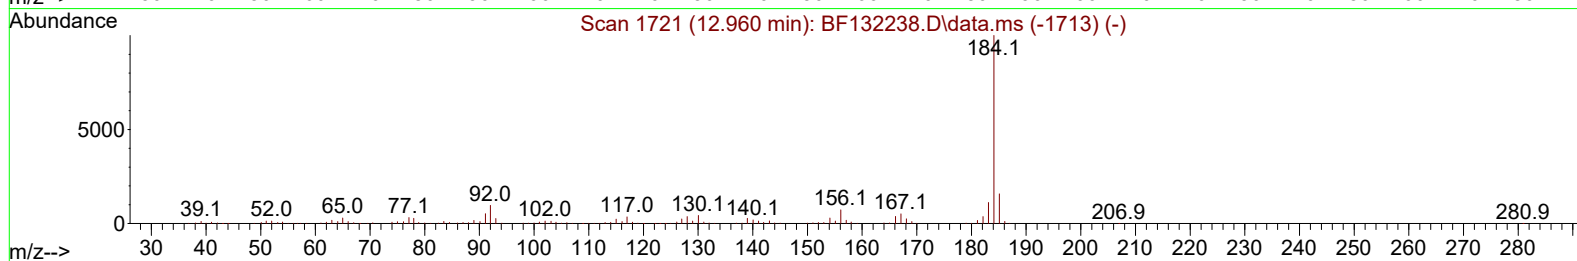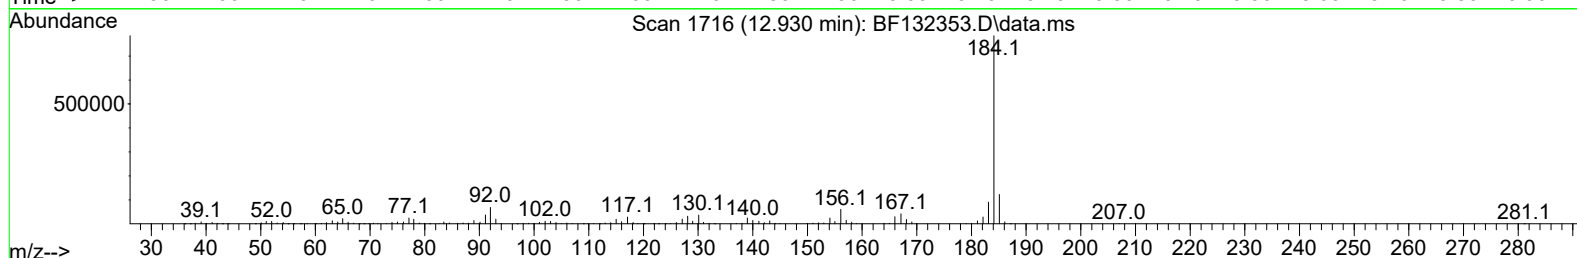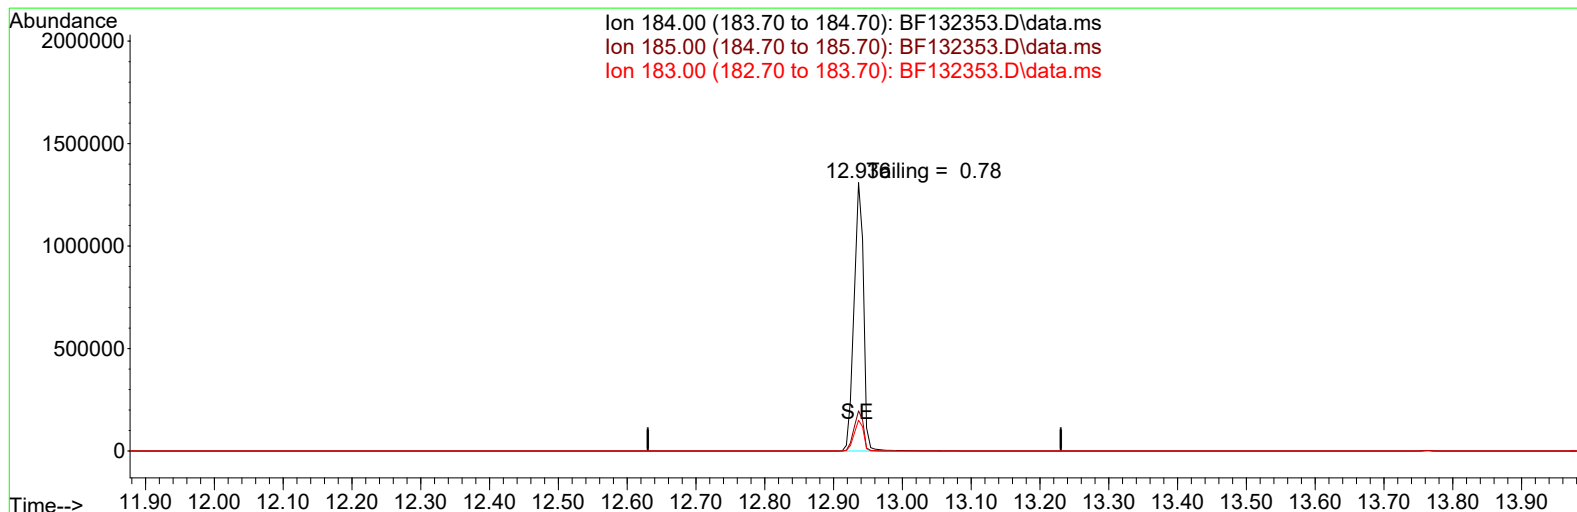

TIC: BF132353.D\data.ms

(77) Benzidine

12.930min (-12.930) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.70	0.00#
183.00	11.10	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2023	BNA_F	<u>BF132353.D</u>
Compound Name	Response	Retention Time
DDT	647107	13.766
DDD	11912	13.46
DDE	769	13.119
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12681	659788	1.92

Instrument :
BNA_F
ClientSampleId :
DFTPP