
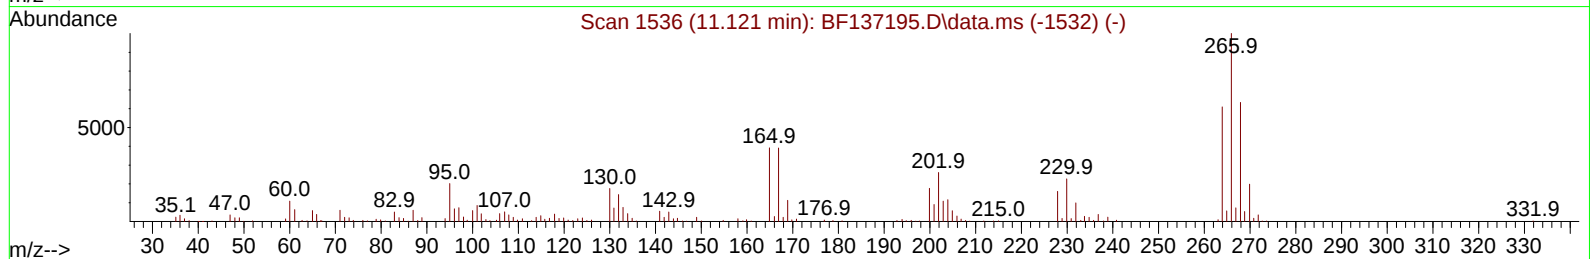
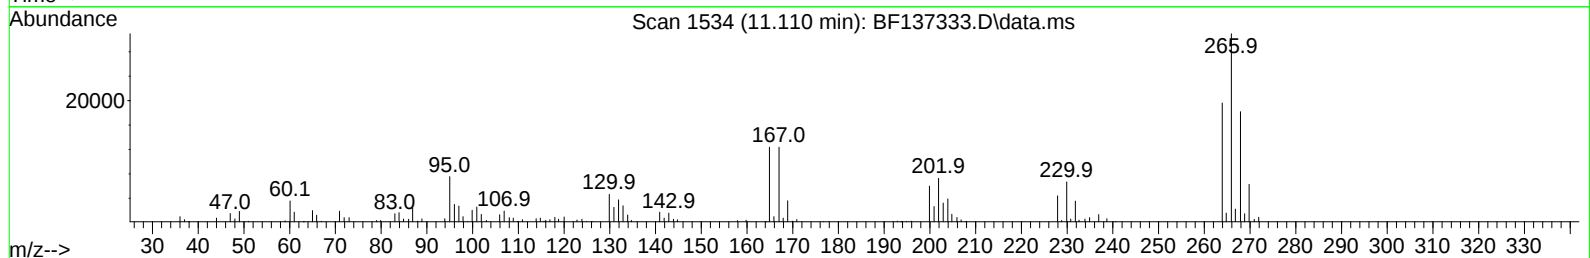


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020824\
Data File : BF137333.D
Acq On : 08 Feb 2024 12:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 13:27:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

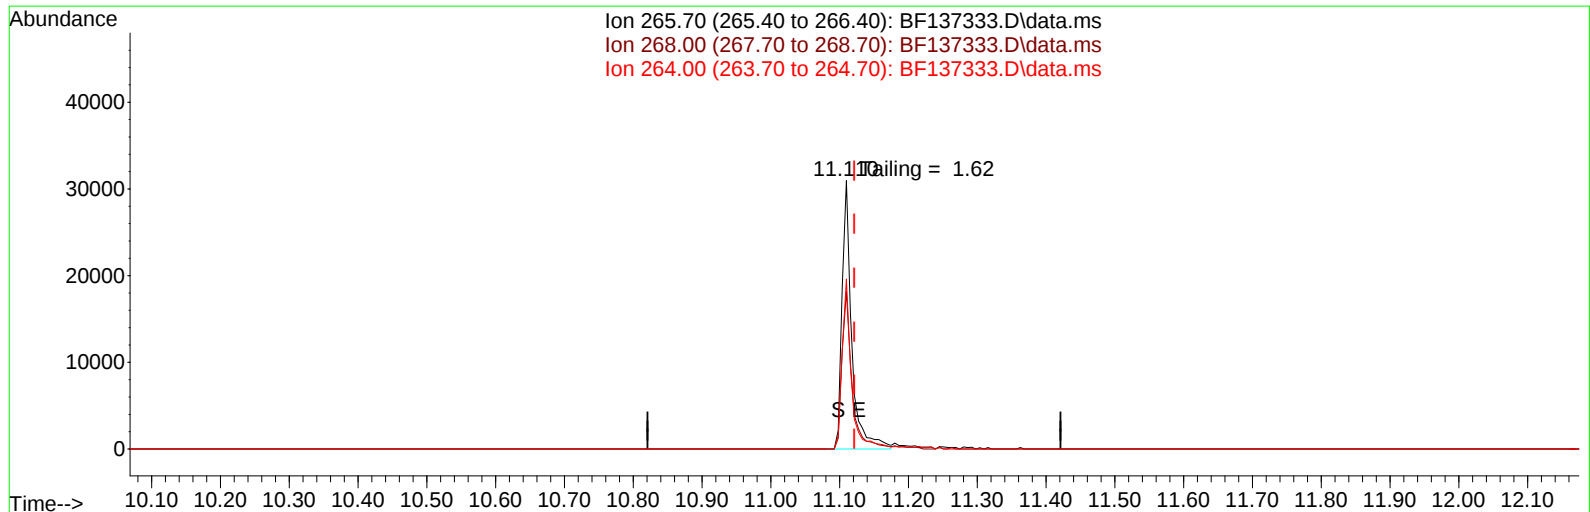

TIC: BF137333.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.011) 39858.71 ng

response 30308

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	58.73
264.00	61.00	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020824\
Data File : BF137333.D
Acq On : 08 Feb 2024 12:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 13:27:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 31 04:56:22 2024
Response via : Initial Calibration

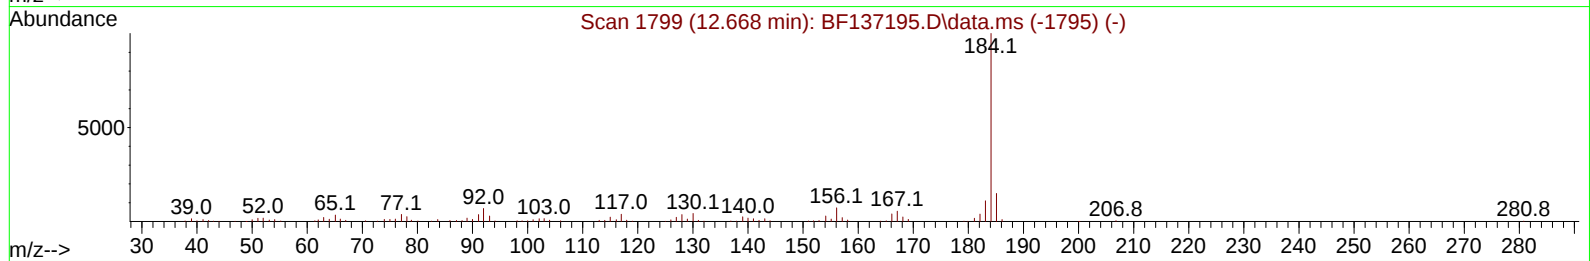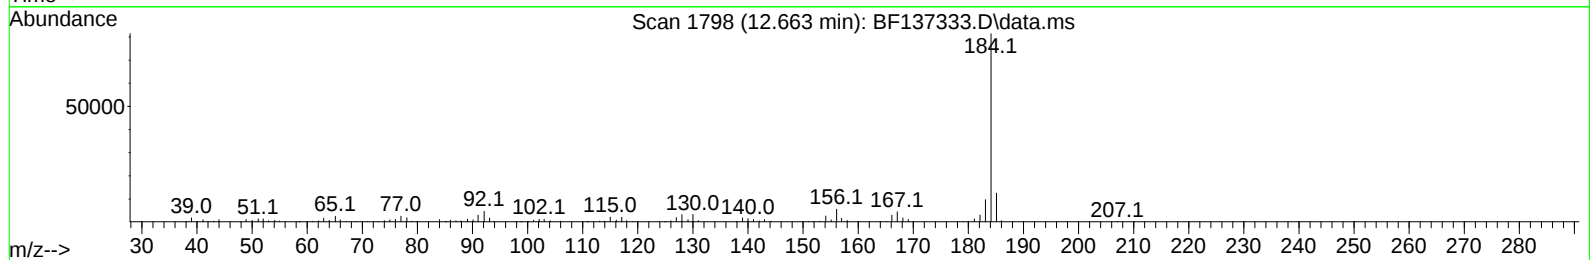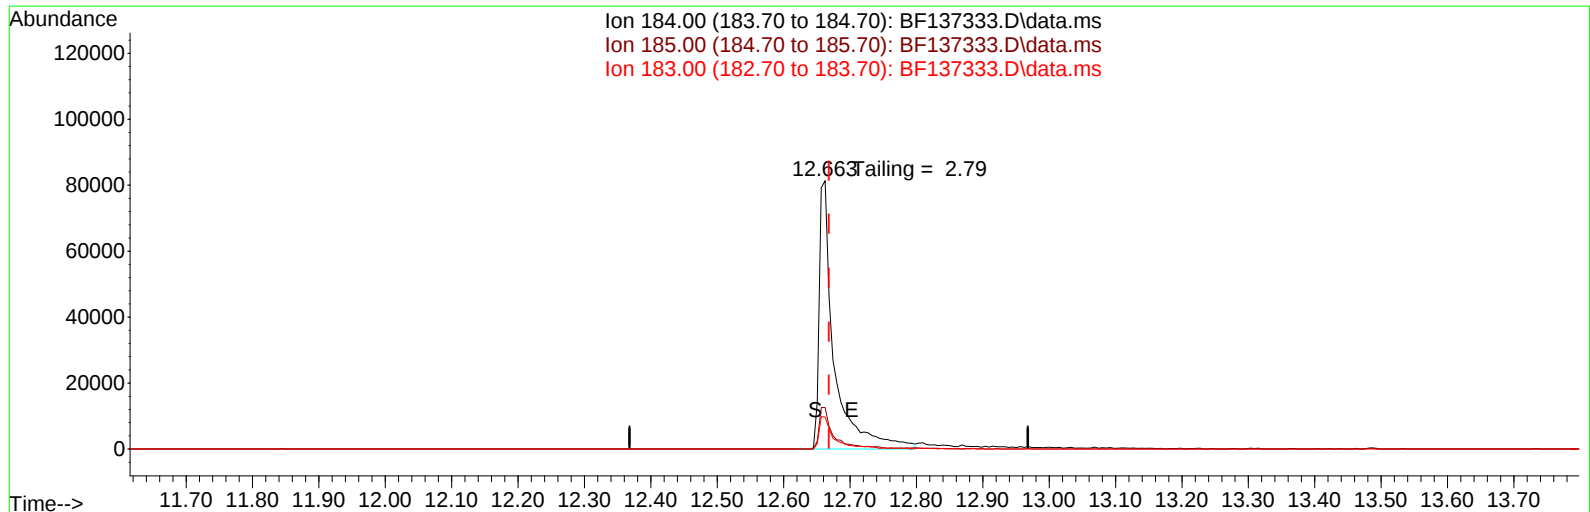

TIC: BF137333.D\data.ms

(77) Benzidine

12.663min (-0.005) 0.00 ng

response 128586

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.43
183.00	11.00	11.92
0.00	0.00	0.00