
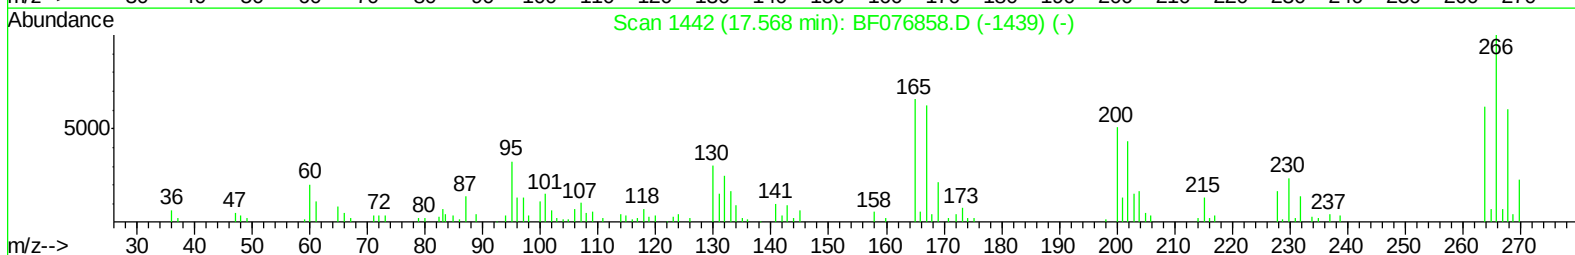
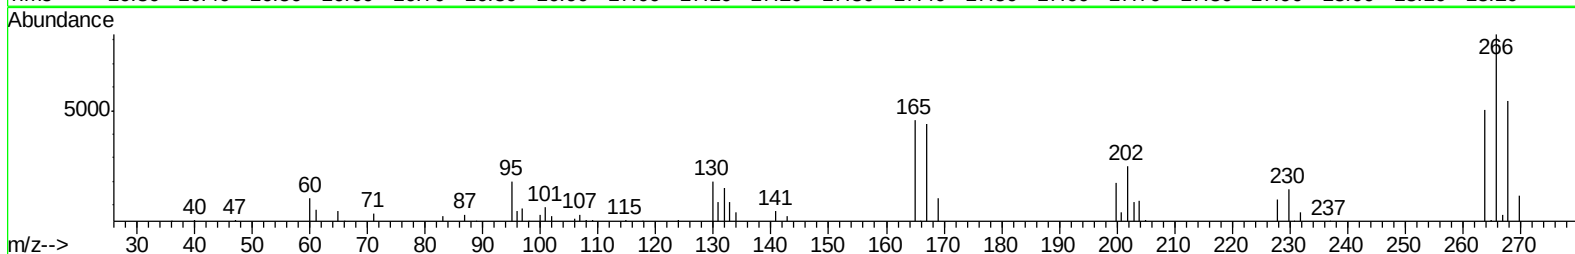


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020915\
Data File : BF077221.D
Acq On : 9 Feb 2015 10:49
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 23:48:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 09 15:41:22 2015
Response via : Initial Calibration

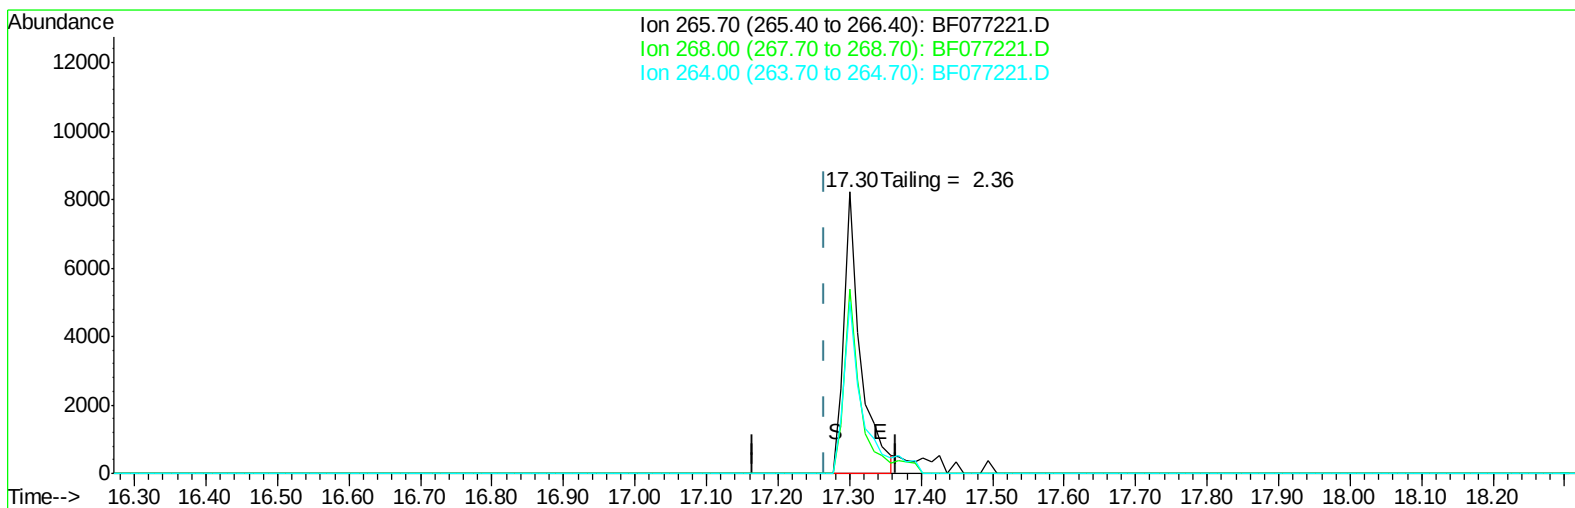

TIC: BF077221.D

(69) Pentachlorophenol (C)




17.300min (+0.034) 0.00ng

response 11545

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.68
264.00	61.90	61.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF020915\
Data File : BF077221.D
Acq On : 9 Feb 2015 10:49
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 23:48:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 09 15:41:22 2015
Response via : Initial Calibration

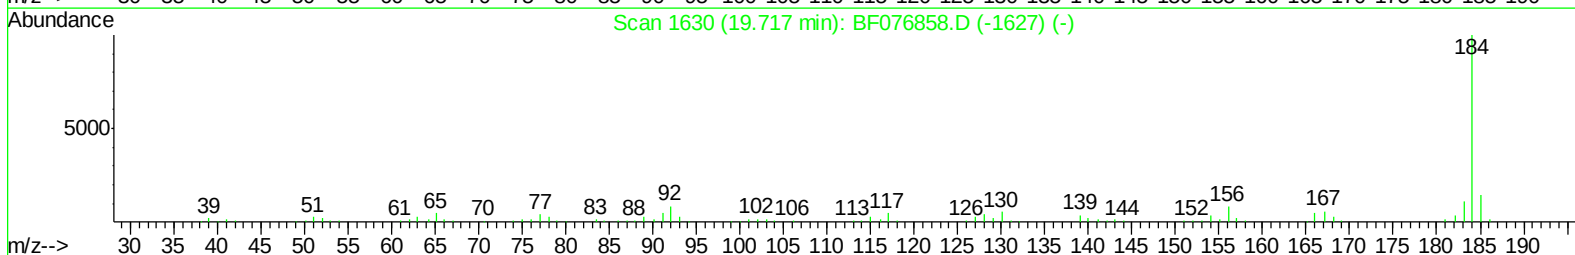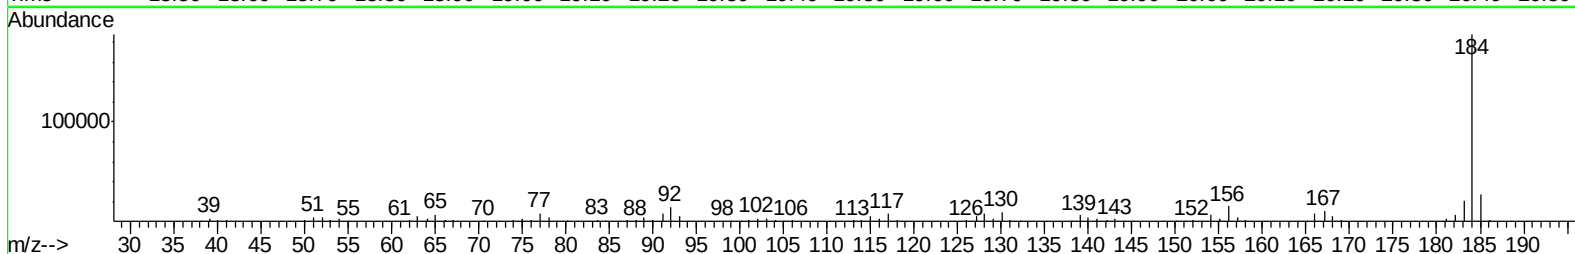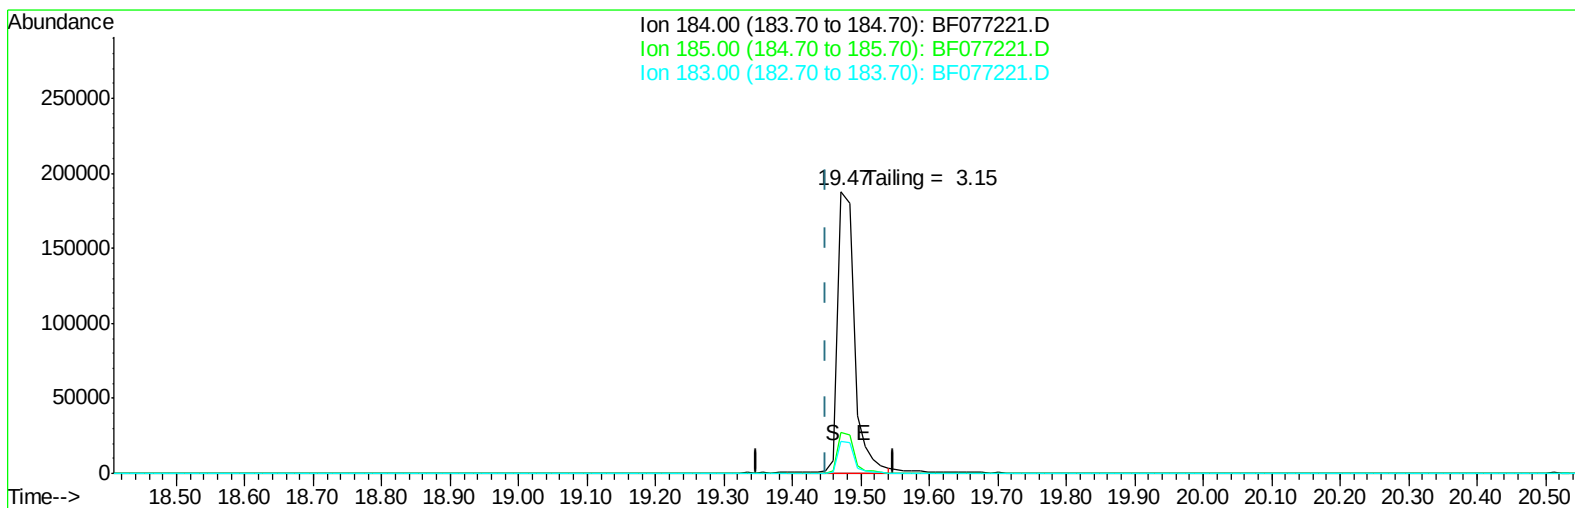

TIC: BF077221.D

(76) Benzidine

19.471min (+0.023) 0.00ng m

response 312045

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.35
183.00	11.30	11.40
0.00	0.00	0.00