

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020915\
 Data File : BF077223.D
 Acq On : 9 Feb 2015 14:20
 Operator : TP/IZ
 Sample : G1252-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CF-ALMASI-05

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	40	41	50	rVB	32062	64911	8.15%	0.938%
2	3.607	235	238	250	rBV	59478	170900	21.47%	2.470%
3	4.590	321	324	345	rBV	288817	647503	81.33%	9.357%
4	7.002	533	535	539	rBV	374898	617657	77.58%	8.926%
5	7.082	539	542	548	rVB	421932	754655	94.79%	10.906%
6	7.596	584	587	595	rVB	91534	163607	20.55%	2.364%
7	7.905	611	614	624	rBV	293797	516651	64.90%	7.466%
8	8.899	698	701	713	rBV	256592	414780	52.10%	5.994%
9	10.499	838	841	852	rVB	139602	230416	28.94%	3.330%
10	13.151	1070	1073	1077	rBV	459739	761574	95.66%	11.006%
11	14.237	1165	1168	1174	rVB	15881	25682	3.23%	0.371%
12	14.614	1198	1201	1208	rVB	156946	250818	31.51%	3.625%
13	16.328	1348	1351	1352	rBV	9782	15752	1.98%	0.228%
14	16.374	1352	1355	1363	rVB	297158	467832	58.77%	6.761%
15	17.506	1451	1454	1457	rBV	206186	269817	33.89%	3.899%
16	18.534	1541	1544	1546	rBV2	5513	8408	1.06%	0.122%
17	19.460	1622	1625	1627	rBV	9130	14398	1.81%	0.208%
18	19.757	1648	1651	1653	rBV	625441	796104	100.00%	11.505%
19	21.014	1758	1761	1769	rVB	280771	345625	43.41%	4.995%
20	21.163	1771	1774	1777	rBV	21032	22476	2.82%	0.325%
21	21.815	1826	1831	1833	rBV2	8851	11728	1.47%	0.169%
22	22.260	1867	1870	1875	rBV	6457	9332	1.17%	0.135%
23	22.580	1895	1898	1903	rBV2	9643	16634	2.09%	0.240%
24	22.695	1906	1908	1915	rVB	176148	238570	29.97%	3.448%
25	22.958	1929	1931	1933	rBV	7104	8931	1.12%	0.129%
26	23.335	1959	1964	1965	rBV	11468	16046	2.02%	0.232%
27	23.358	1965	1966	1972	rVV2	9651	20412	2.56%	0.295%
28	23.712	1994	1997	2001	rBV4	7192	15687	1.97%	0.227%
29	24.089	2026	2030	2032	rBV2	6214	13440	1.69%	0.194%
30	24.146	2032	2035	2039	rVB3	4411	9550	1.20%	0.138%


Sum of corrected areas: 6919896

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020915\
Data File : BF077223.D
Acq On : 9 Feb 2015 14:20
Operator : TP/IZ
Sample : G1252-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-ALMASI-05

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

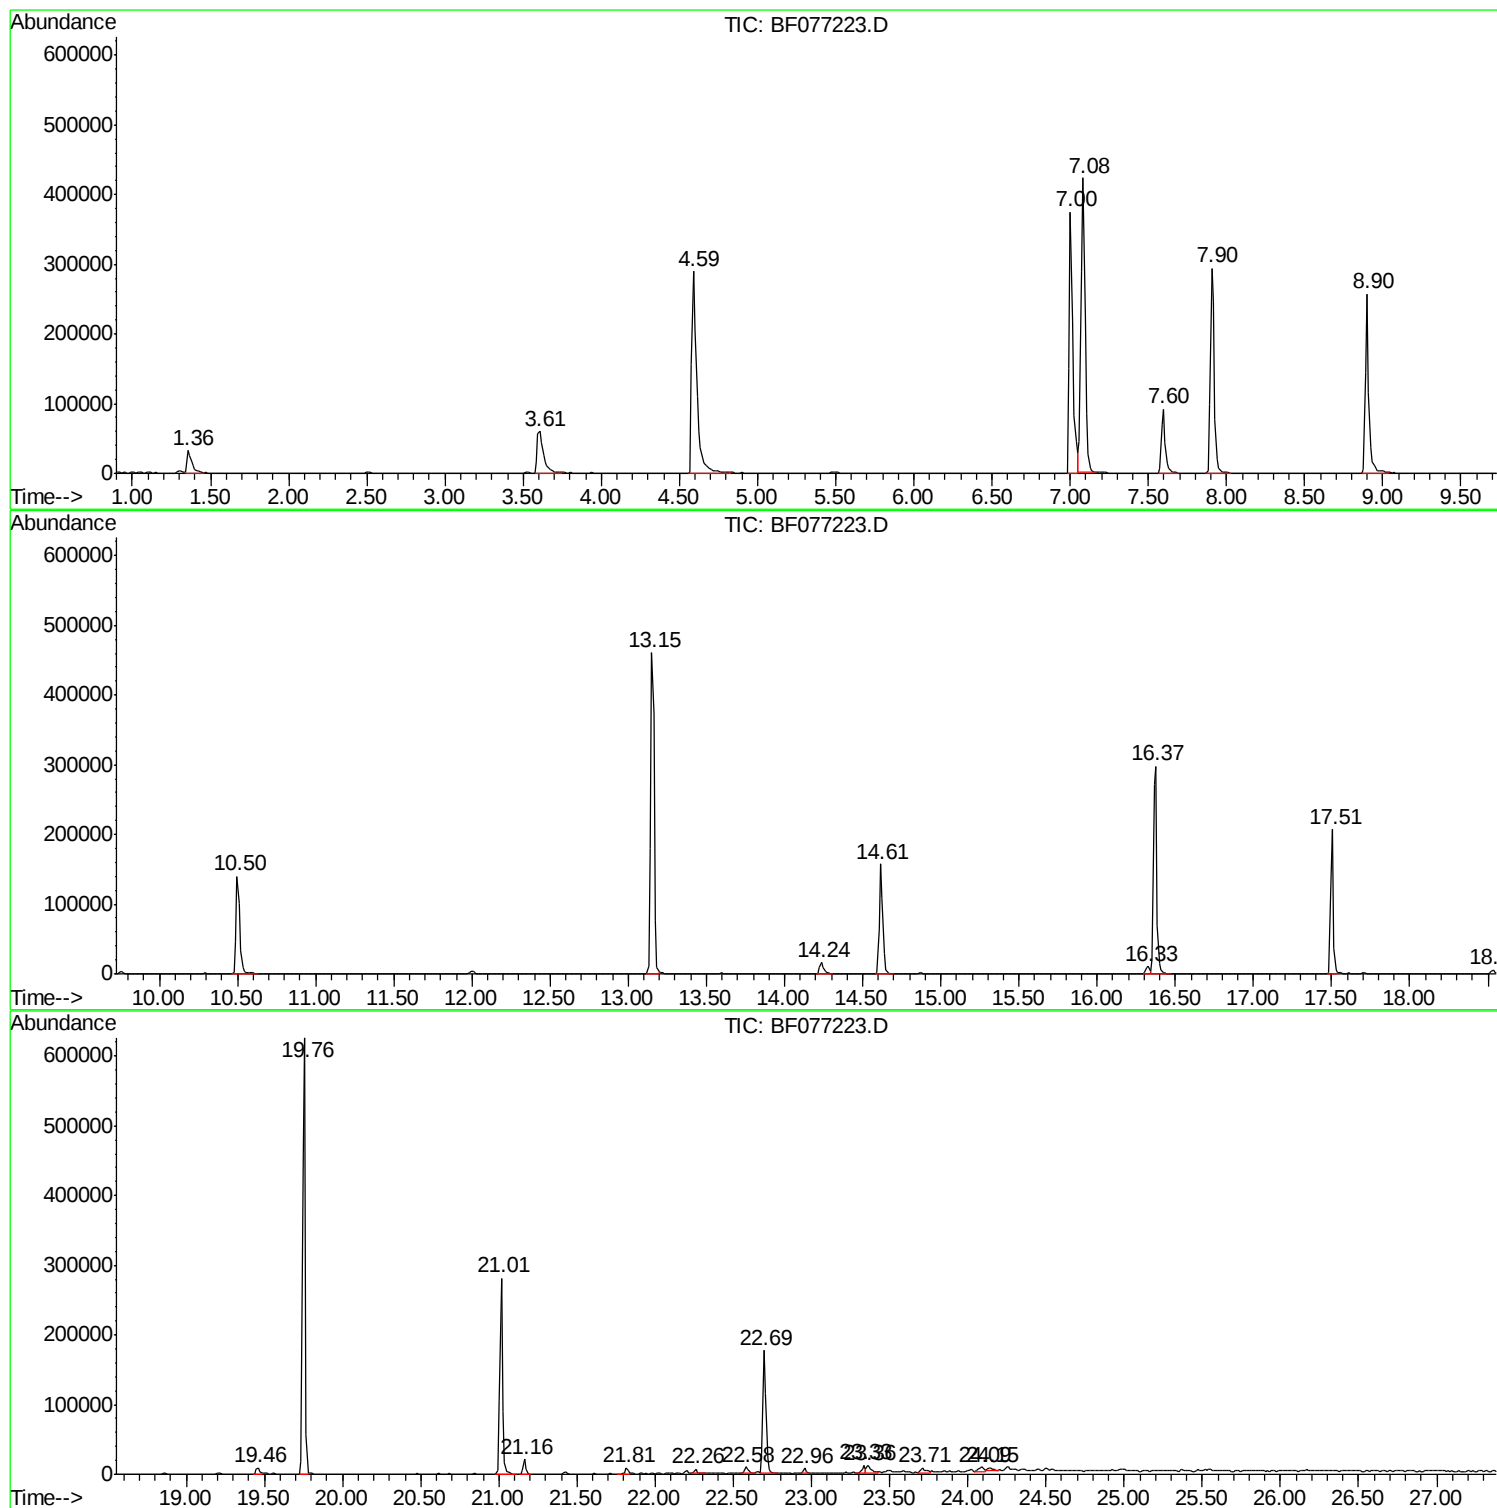

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020915\
Data File : BF077223.D
Acq On : 9 Feb 2015 14:20
Operator : TP/IZ
Sample : G1252-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-ALMASI-05










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.61	20.89 ng	170900	1,4-Dichlorobenzene-d4	7.60

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			Guanidine	59	CH5N3	000113-00-8	47
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	36
4			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	28

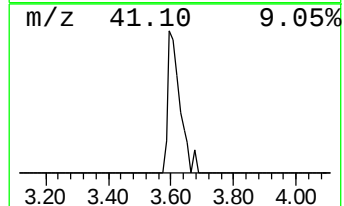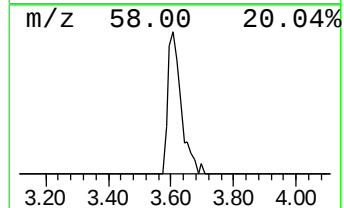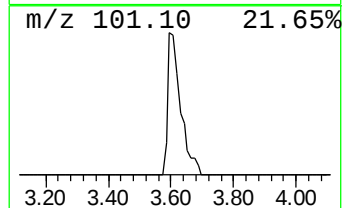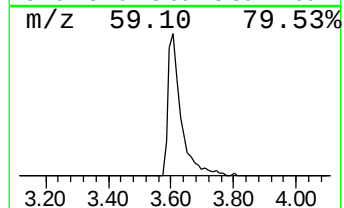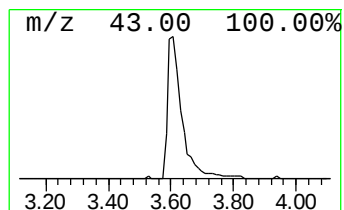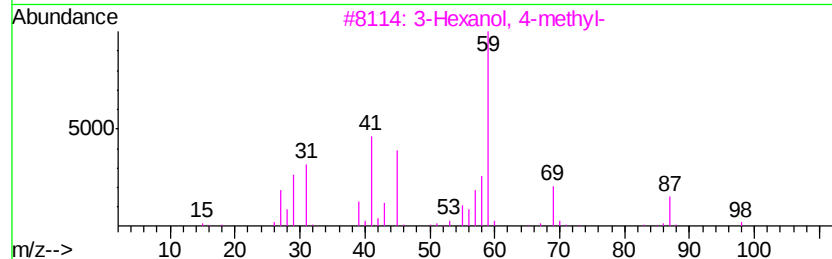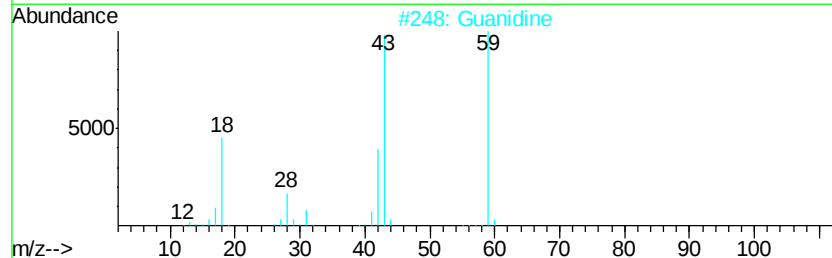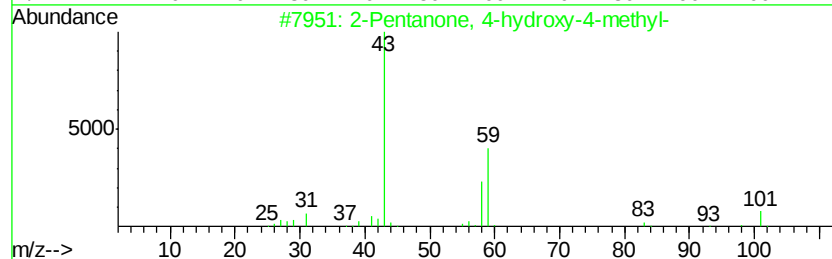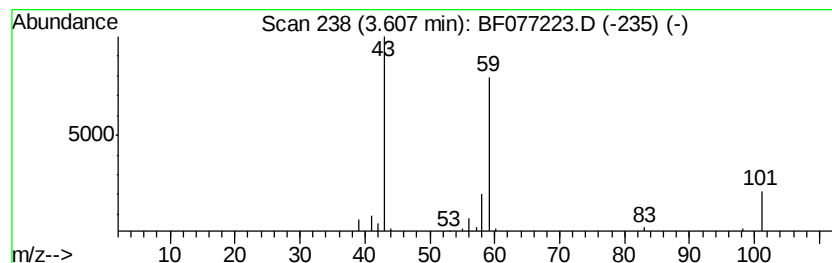

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020915\
Data File : BF077223.D
Acq On : 9 Feb 2015 14:20
Operator : TP/IZ
Sample : G1252-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CF-ALMASI-05

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	3.61	20.9	ng	170900	1	7.60	163607	20.0