


Data Path : Z:\HPCHEM1\BNA_F\Data\BF020915\
 Data File : BF077221.D
 Acq On : 9 Feb 2015 12:29
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 09 15:41:22 2015

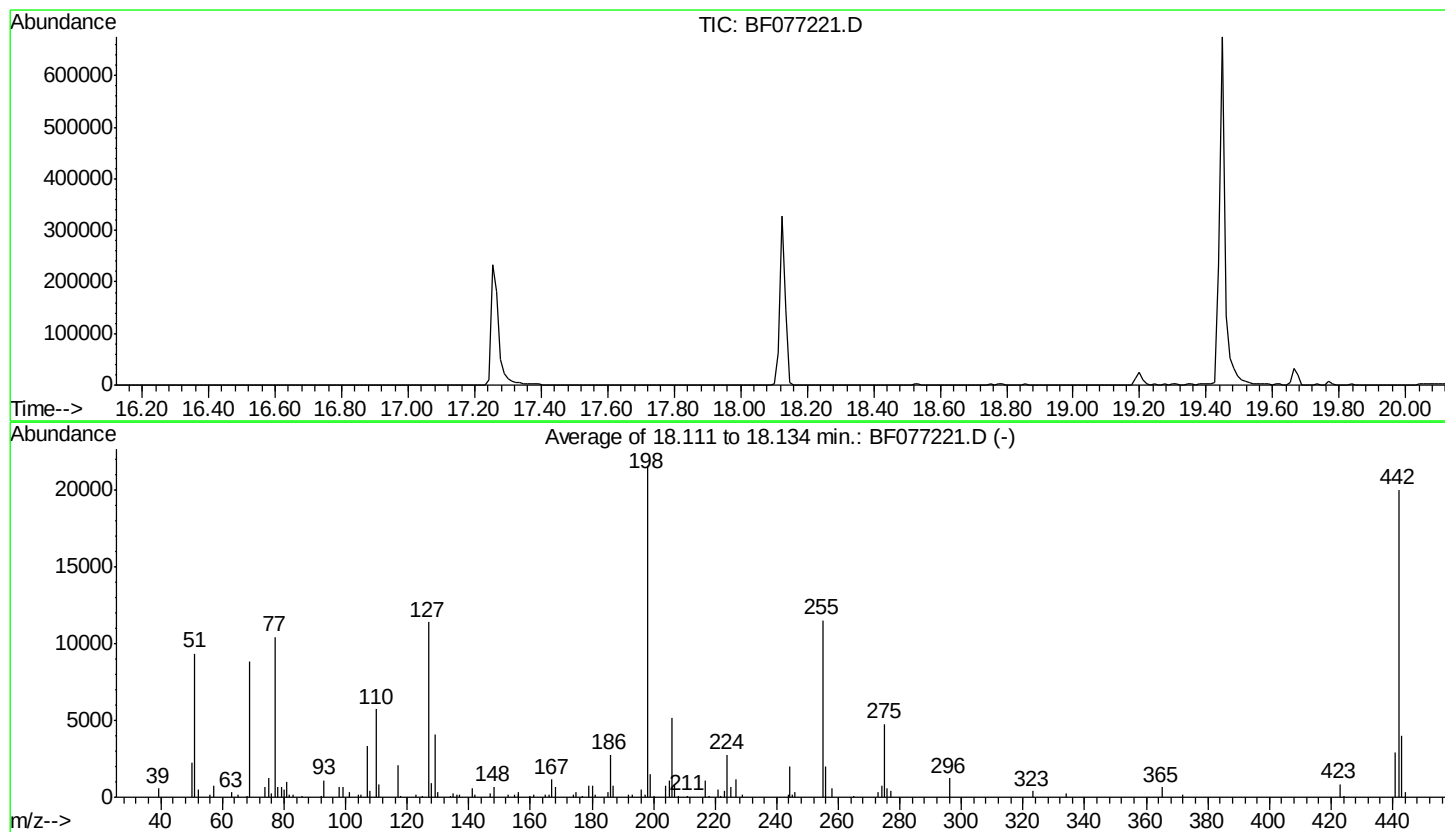

AutoFind: Scans 1507, 1508, 1509; Background Corrected with Scan 1504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	9352	PASS
68	69	0.00	2	1.3	114	PASS
69	198	0.00	100	41.0	8847	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.9	11403	PASS
197	198	0.00	2	0.6	138	PASS
198	198	100	100	100.0	21567	PASS
199	198	5	9	7.0	1504	PASS
275	198	10	60	22.2	4778	PASS
365	198	1	100	3.0	657	PASS
441	442	0.01	24	14.4	2889	PASS
442	198	50	100	92.8	20023	PASS
443	442	15	24	20.1	4015	PASS