

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
 Data File : BF084978.D
 Acq On : 10 Feb 2016 3:22
 Operator : SJ/IZ
 Sample : H1386-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)

Quant Time: Feb 10 05:47:58 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 03 14:16:01 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.64	152	163567	20.00	ng	-0.05
21) Naphthalene-d8	7.92	136	621796	20.00	ng	-0.06
38) Acenaphthene-d10	9.66	164	275241	20.00	ng	-0.07
63) Phenanthrene-d10	11.14	188	455819	20.00	ng	-0.07
75) Chrysene-d12	13.77	240	307456	20.00	ng	-0.07
86) Perylene-d12	15.14	264	286203	20.00	ng	-0.07

System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	223347	21.27	ng	-0.06
7) Phenol-d6	6.28	99	1242786	95.46	ng	-0.06
23) Nitrobenzene-d5	7.21	82	953687	86.40	ng	-0.06
41) 2,4,6-Tribromophenol	10.45	330	10164	3.54	ng	-0.07
44) 2-Fluorobiphenyl	9.00	172	1453438	91.13	ng	-0.06
78) Terphenyl-d14	12.73	244	937434	69.09	ng	-0.07


Target Compounds						Qvalue
19) n-Nitroso-di-n-propylamine	7.21	70	133410	16.35	ng	# 75
49) Dimethylphthalate	9.40	163	302011	14.41	ng	# 90
51) Acenaphthene	9.70	154	51101	2.86	ng	96
54) Dibenzofuran	9.87	168	53807	2.46	ng	# 96
60) 4-Chlorophenyl-phenylether	10.04	204	1295	Below	Cal	# 57
70) Phenanthrene	11.17	178	602476	23.83	ng	100
71) Anthracene	11.22	178	163007	6.40	ng	98
72) Carbazole	11.38	167	61654	2.78	ng	99
74) Fluoranthene	12.35	202	610511	23.86	ng	98
76) Benzidine	12.51	184	593	6.93	ng	# 1
77) Pyrene	12.58	202	543976	23.11	ng	99
80) Benzo(a)anthracene	13.77	228	235969	12.37	ng	98
82) Chrysene	13.77	228	235969	12.75	ng	98
83) Bis(2-ethylhexyl)phthalate	13.78	149	31258	2.35	ng	# 84
85) Indeno(1,2,3-cd)pyrene	16.40	276	95549	6.56	ng	92
87) Benzo(b)fluoranthene	14.77	252	305904	15.91	ng	# 93
88) Benzo(k)fluoranthene	14.77	252	305904	19.24	ng	97
89) Benzo(a)pyrene	15.08	252	165130	10.08	ng	# 90
91) Benzo(g,h,i)perylene	16.77	276	88518	6.37	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
Data File : BF084978.D
Acq On : 10 Feb 2016 3:22
Operator : SJ/IZ
Sample : H1386-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S4-B005(0-2)

Quant Time: Feb 10 05:47:58 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 03 14:16:01 2016
Response via : Initial Calibration

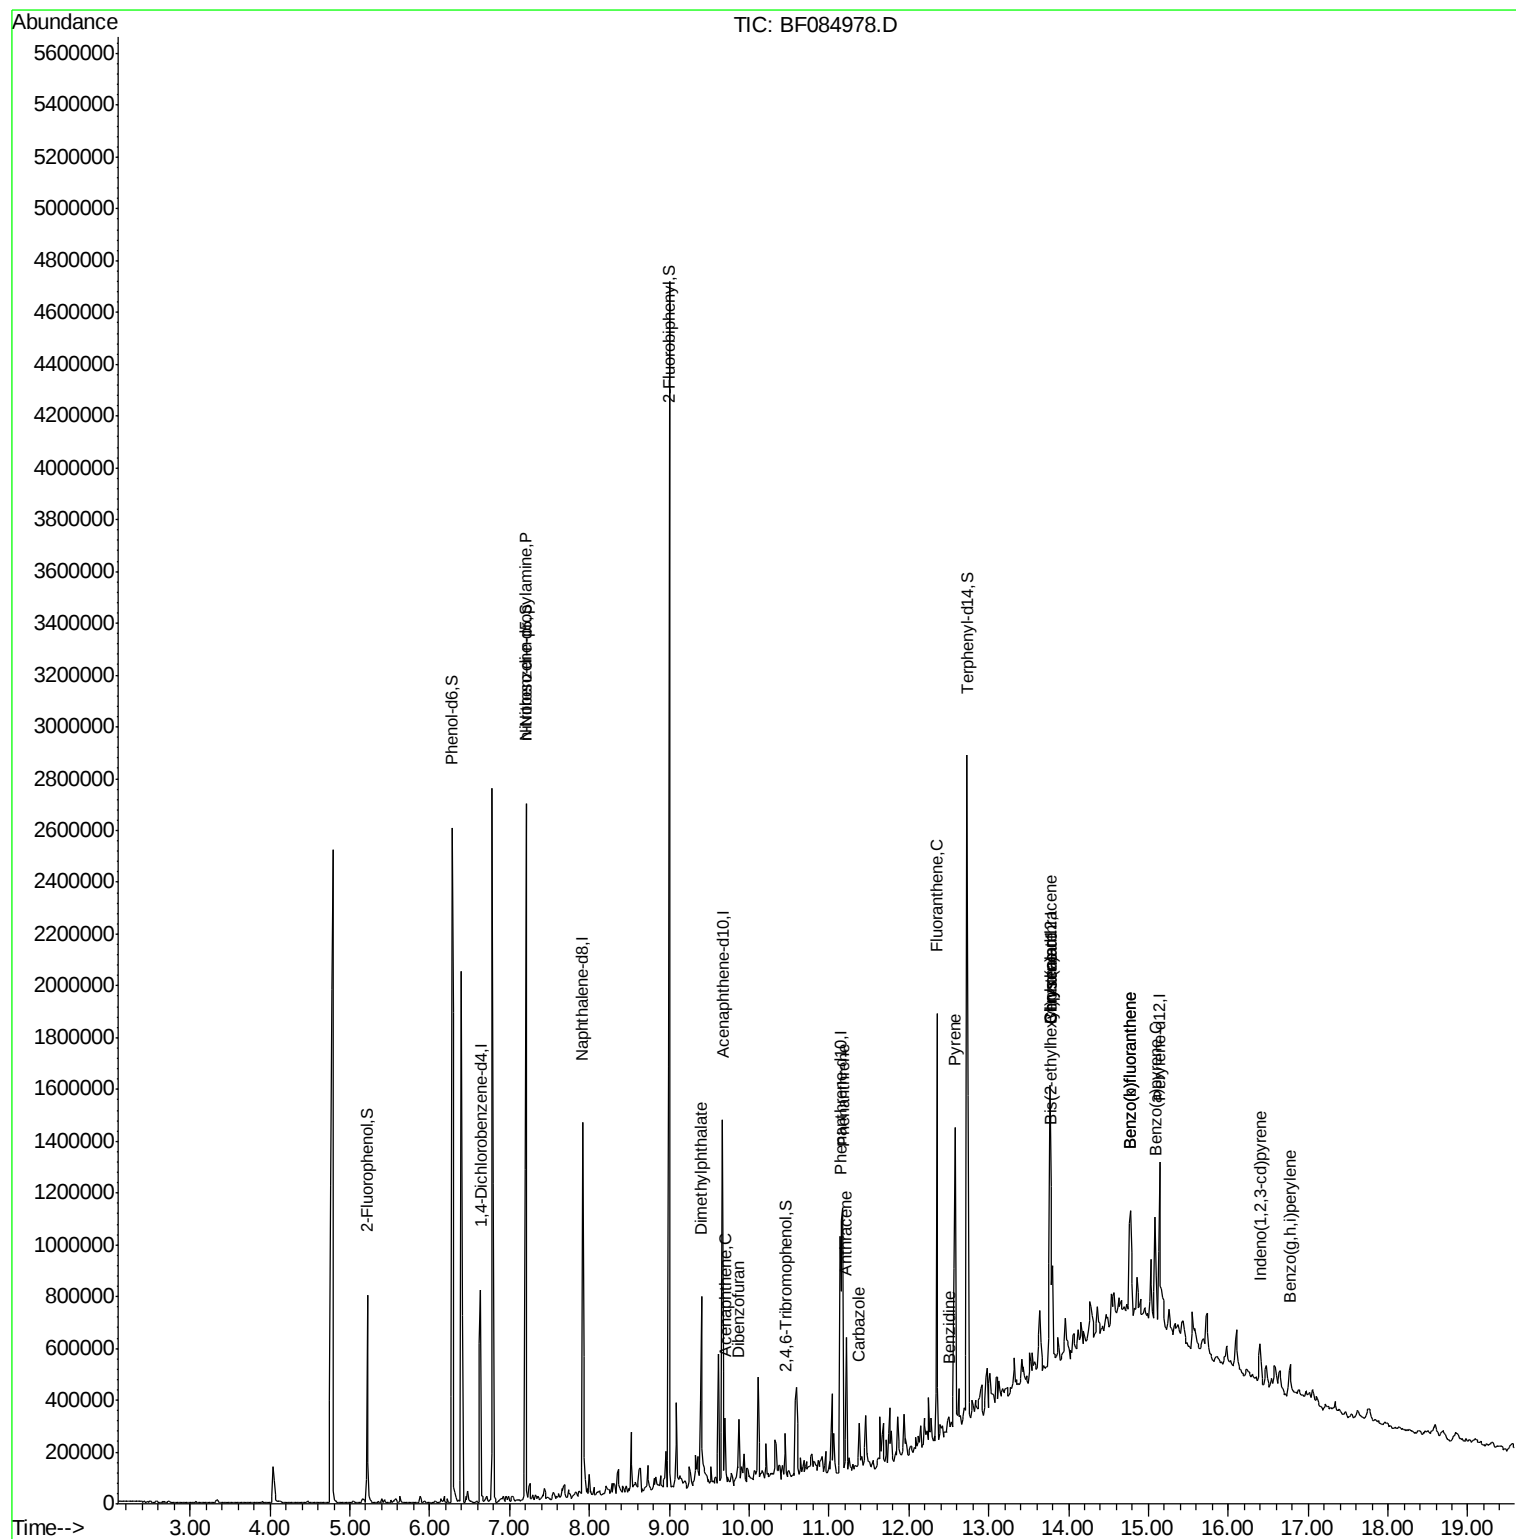

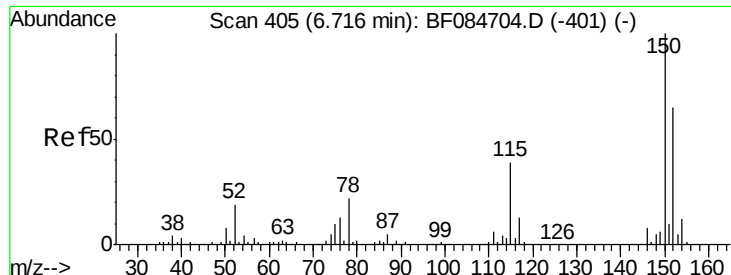

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.64 min Scan# 398

Delta R.T. -0.05 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:152 Resp: 163567

Ion Ratio Lower Upper

152 100

150 152.1 123.0 184.4




115 55.5 51.4 77.2

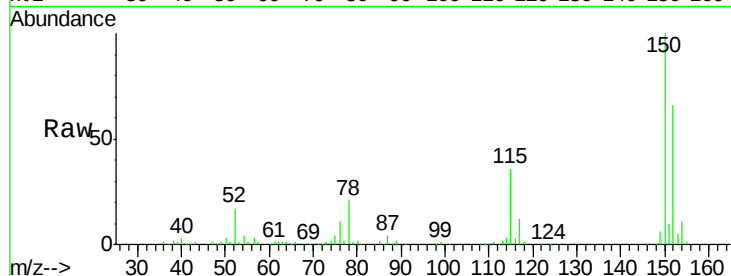

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

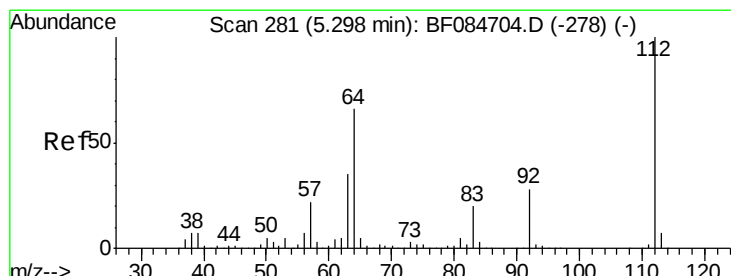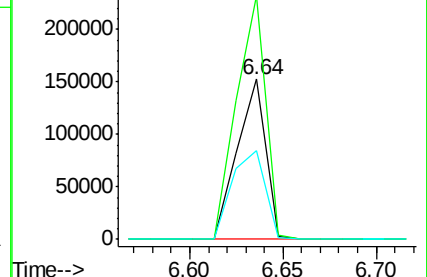

#5

2-Fluorophenol

Concen: 21.27 ng

RT: 5.22 min Scan# 274

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:112 Resp: 223347

Ion Ratio Lower Upper

112 100

64 58.5 36.6 55.0#



63 29.1 19.4 29.0#

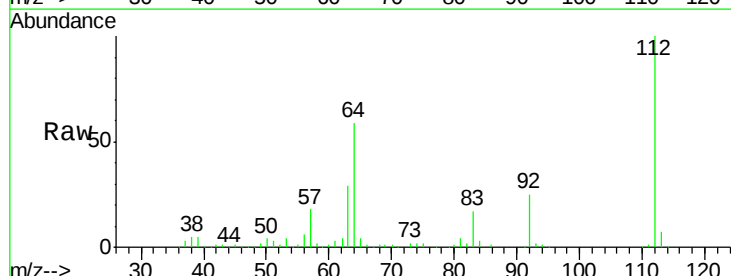


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

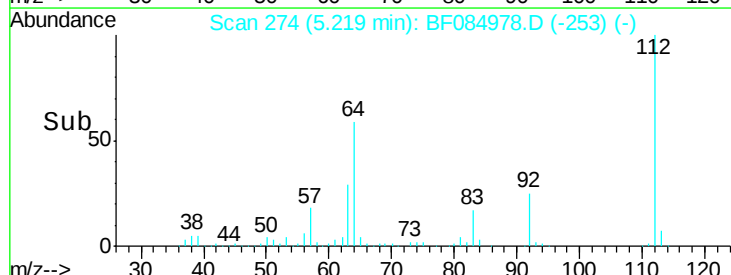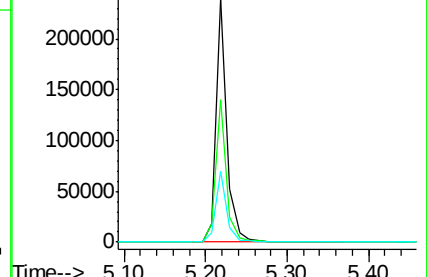

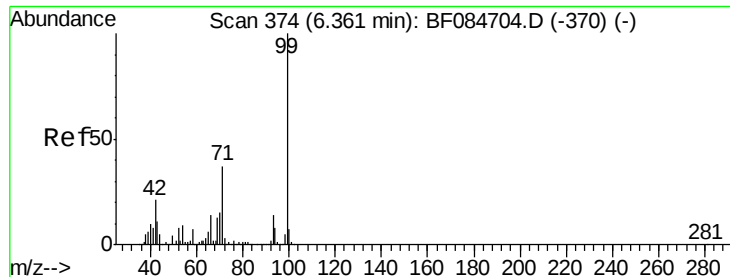

#7

Phenol-d6

Concen: 95.46 ng

RT: 6.28 min Scan# 367

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion: 99 Resp: 1242786

Ion Ratio Lower Upper

99 100

42 20.9 12.8 19.2#




71 37.2 30.9 46.3

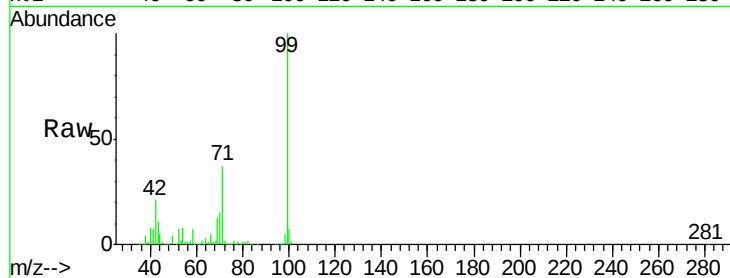

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

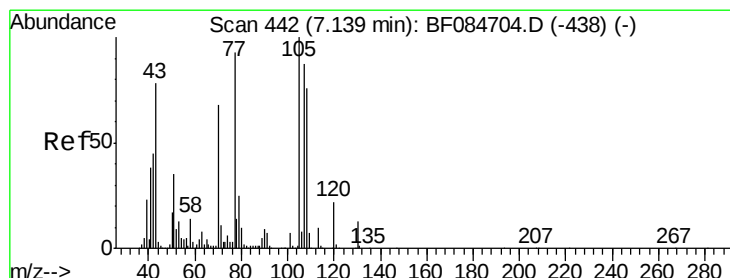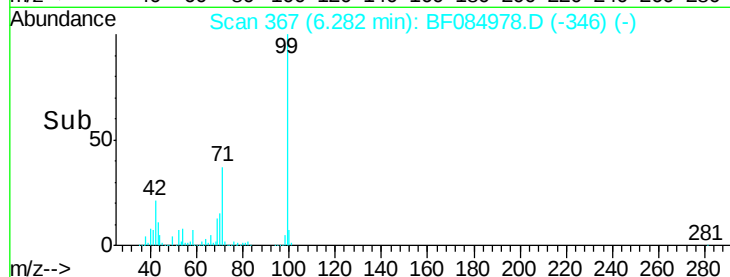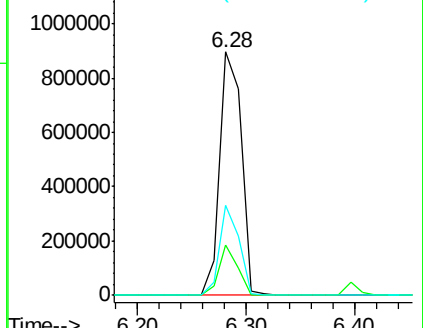

#19

n-Nitroso-di-n-propylamine

Concen: 16.35 ng

RT: 7.21 min Scan# 448

Delta R.T. 0.09 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Tgt Ion: 70 Resp: 133410


Ion Ratio Lower Upper

70 100

42 45.9 33.3 49.9

101 0.0 9.3 13.9#

130 2.4 23.4 35.0#


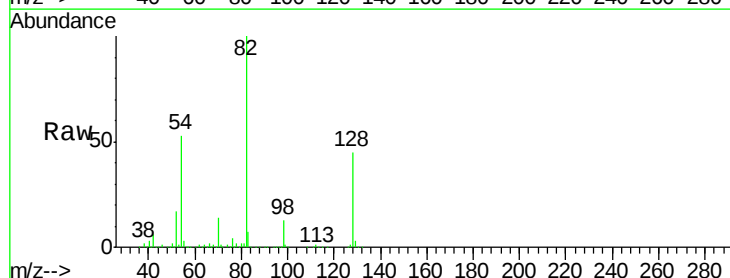



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

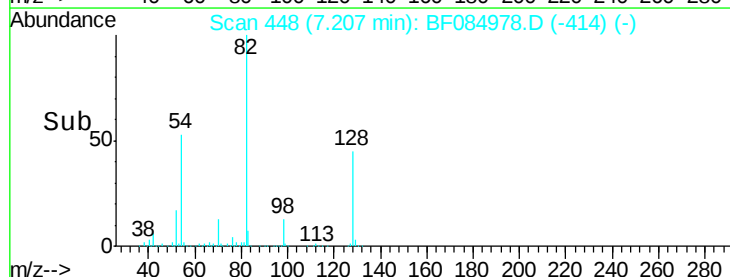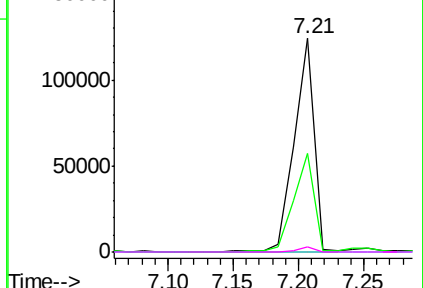

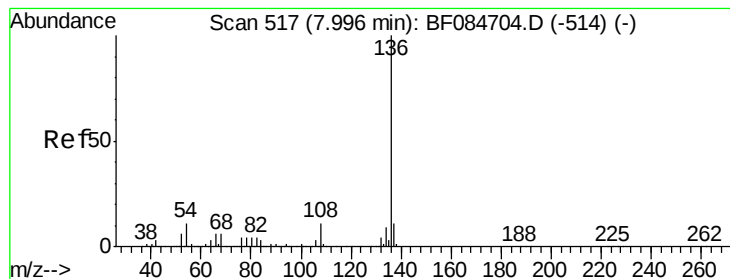

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.92 min Scan# 510

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)

Tgt Ion: 136 Resp: 621796


Ion Ratio Lower Upper

136 100

137 11.3 8.7 13.1

54 10.6 5.8 8.8#

68 5.9 4.2 6.2



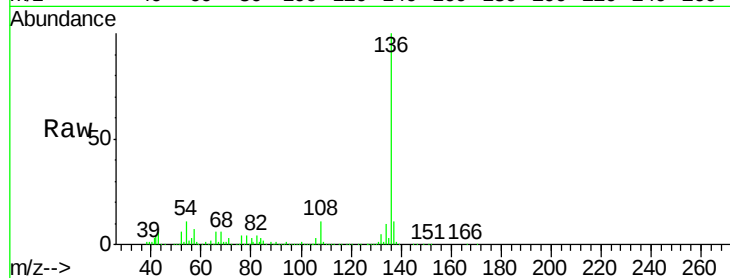


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

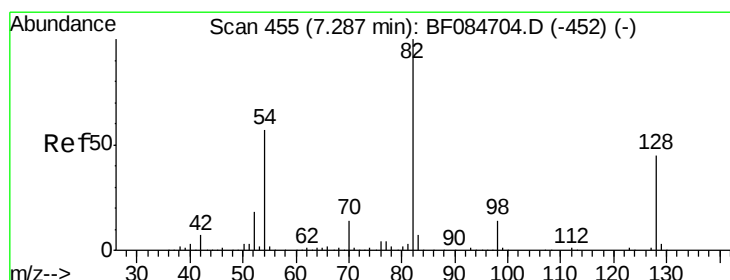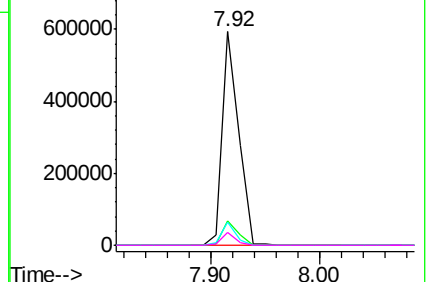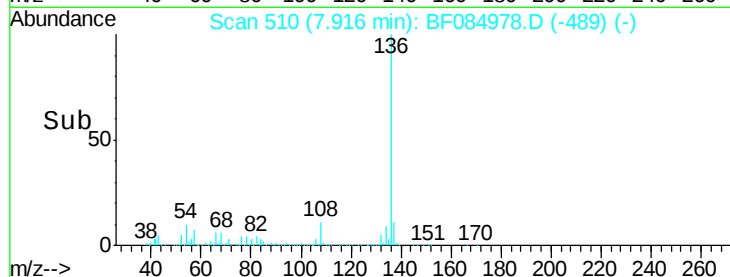

#23

Nitrobenzene-d5

Concen: 86.40 ng

RT: 7.21 min Scan# 448

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion: 82 Resp: 953687

Ion Ratio Lower Upper

82 100

128 45.4 34.6 51.8



54 53.3 38.4 57.6

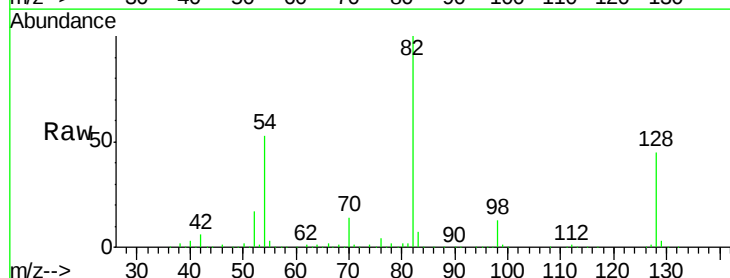


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

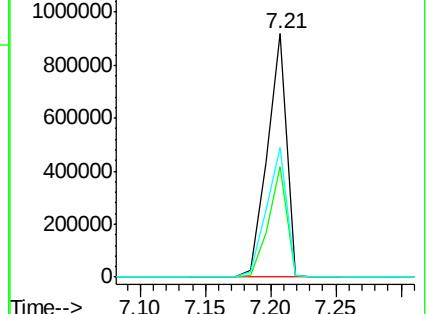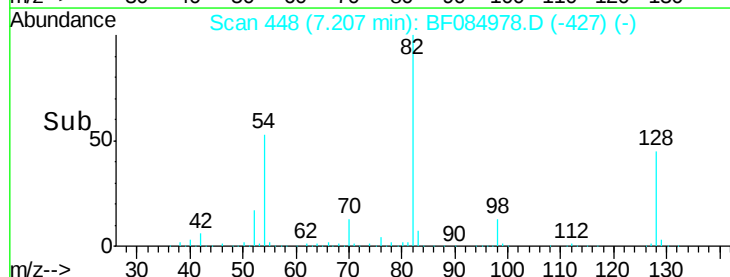







#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.66 min Scan# 663
 Delta R.T. -0.07 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)

Tgt Ion:164 Resp: 275241
 Ion Ratio Lower Upper
 164 100
 162 103.3 85.1 127.7
 160 46.9 37.5 56.3

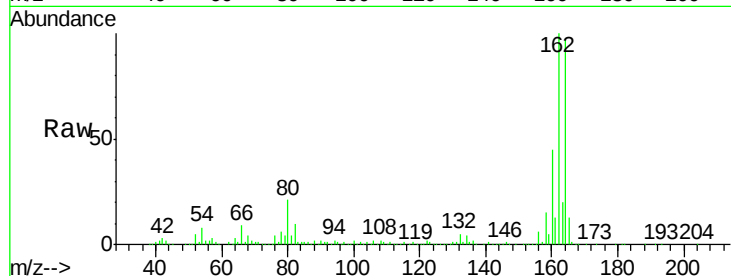


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


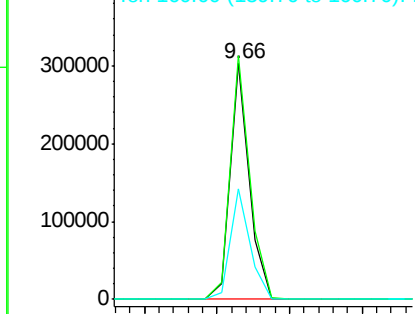



#41
 2,4,6-Tribromophenol
 Concen: 3.54 ng
 RT: 10.45 min Scan# 732
 Delta R.T. -0.07 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Tgt Ion:330 Resp: 10164
 Ion Ratio Lower Upper
 330 100
 332 107.2 76.6 114.8
 141 48.0 27.8 41.6#



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E




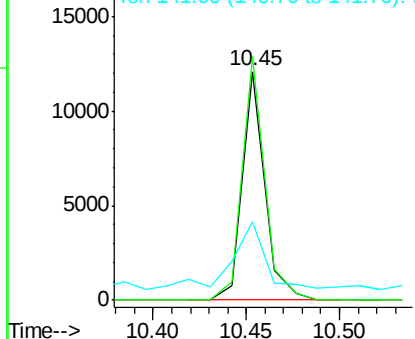




#44
 2-Fluorobiphenyl
 Concen: 91.13 ng
 RT: 9.00 min Scan# 605
 Delta R.T. -0.06 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22




Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)


Tgt Ion:172 Resp: 1453438
 Ion Ratio Lower Upper
 172 100
 171 37.2 28.9 43.3
 170 25.0 18.6 27.8

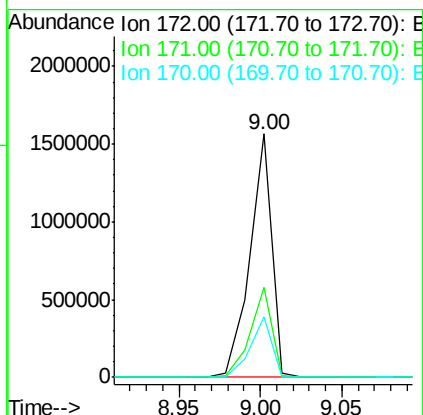

#49
 Dimethylphthalate
 Concen: 14.41 ng
 RT: 9.40 min Scan# 640
 Delta R.T. -0.07 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Tgt Ion:163 Resp: 302011
 Ion Ratio Lower Upper
 163 100
 194 3.4 8.0 12.0#
 164 9.2 8.0 12.0

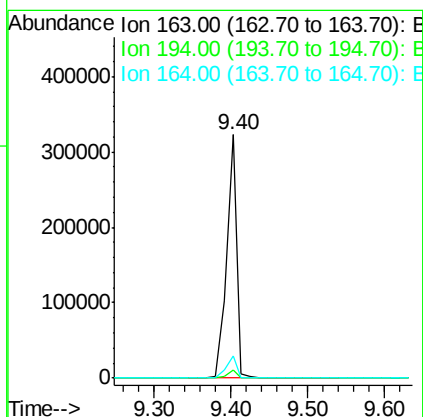

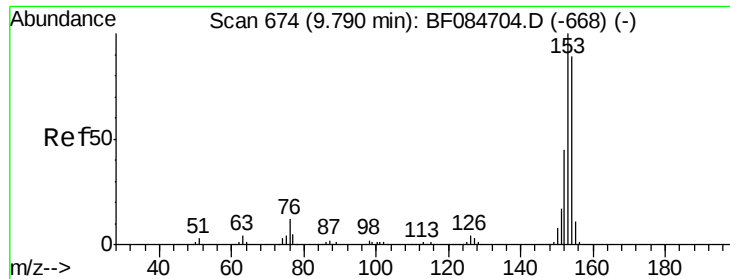

#51

Acenaphthene

Concen: 2.86 ng

RT: 9.70 min Scan# 666

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:154 Resp: 51101

Ion Ratio Lower Upper

154 100

153 110.7 91.5 137.3




152 49.8 43.0 64.6

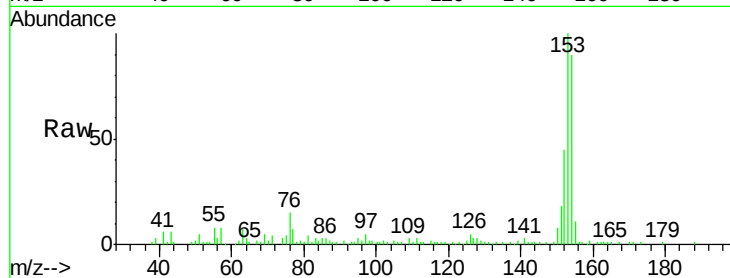

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

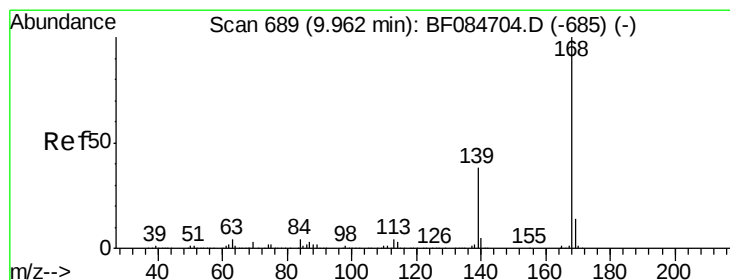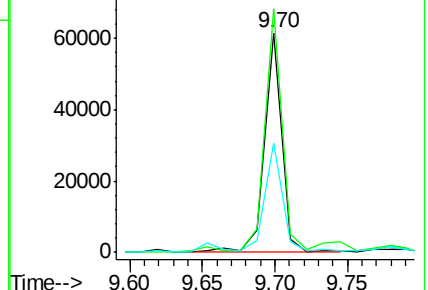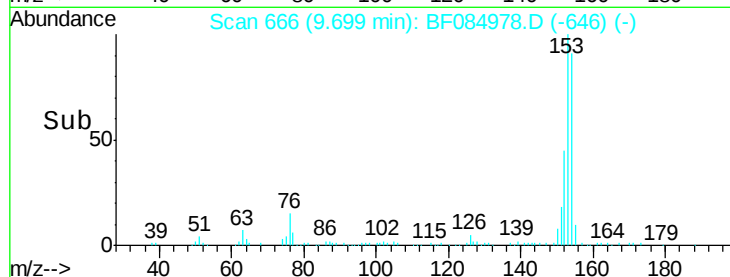

#54

Dibenzofuran

Concen: 2.46 ng

RT: 9.87 min Scan# 681

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:168 Resp: 53807

Ion Ratio Lower Upper

168 100

139 37.5 30.5 45.7



169 17.8 10.4 15.6#

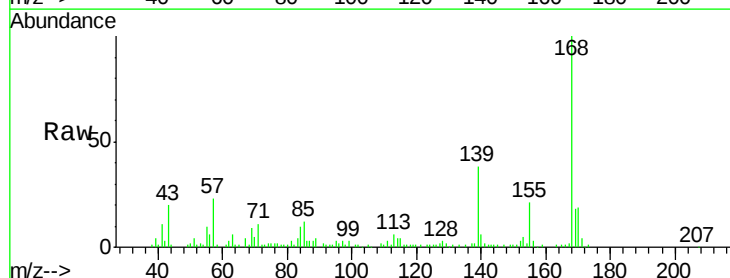


Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E



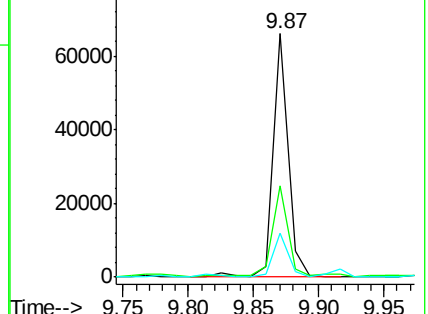
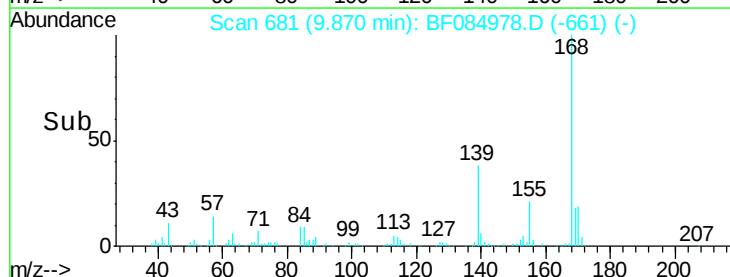


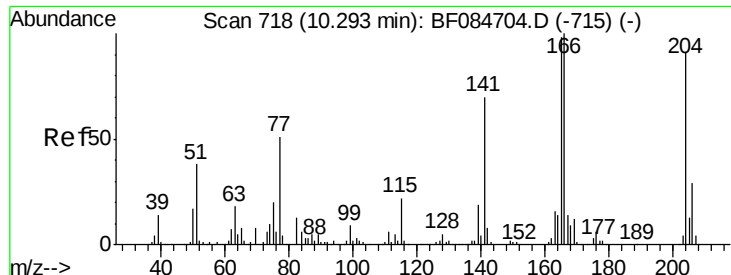

#60
 4-Chlorophenyl-phenylether
 Concen: Below Cal
 RT: 10.04 min Scan# 696
 Delta R.T. -0.23 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22




Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)


Tgt Ion: 204 Resp: 1295
 Ion Ratio Lower Upper
 204 100
 206 0.0 25.7 38.5#
 141 98.2 55.1 82.7#

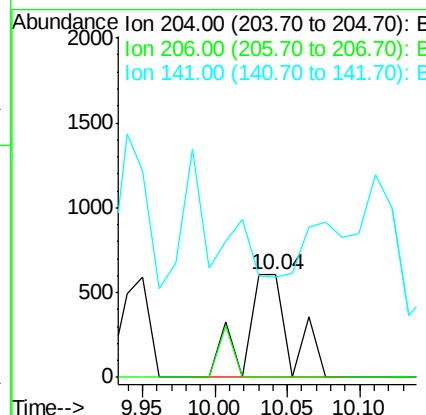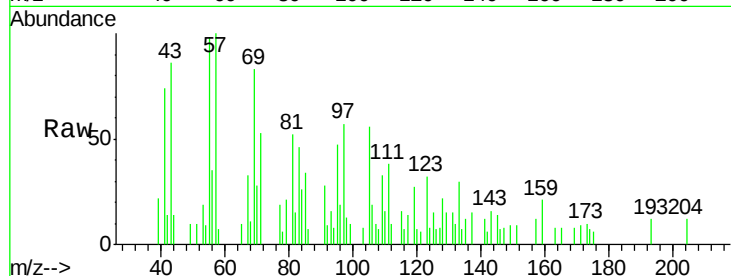

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.14 min Scan# 792
 Delta R.T. -0.07 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Tgt Ion: 188 Resp: 455819
 Ion Ratio Lower Upper
 188 100
 94 11.6 9.0 13.4
 80 12.7 9.6 14.4



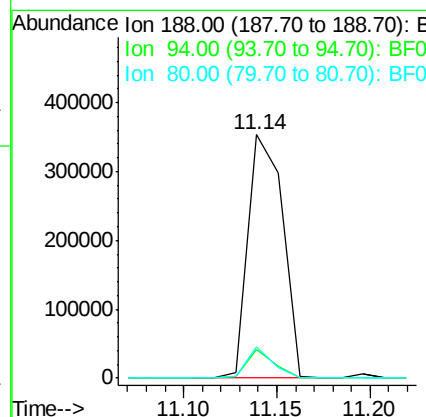





#70
 Phenanthrene
 Concen: 23.83 ng
 RT: 11.17 min Scan# 795
 Delta R.T. -0.06 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22




Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)


Tgt Ion:178 Resp: 602476
 Ion Ratio Lower Upper
 178 100
 176 19.0 15.3 22.9
 179 14.9 12.0 18.0

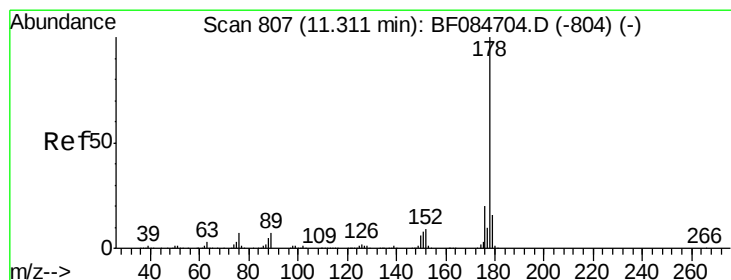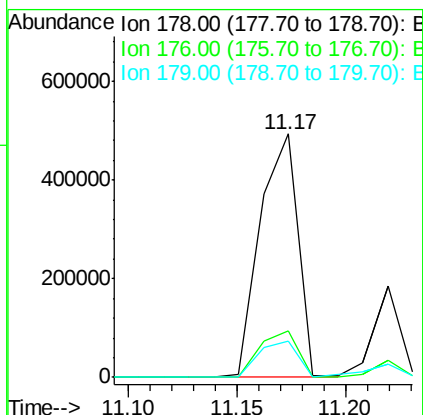

#71
 Anthracene
 Concen: 6.40 ng
 RT: 11.22 min Scan# 799
 Delta R.T. -0.07 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Tgt Ion:178 Resp: 163007
 Ion Ratio Lower Upper
 178 100
 176 17.9 15.4 23.0
 179 15.0 12.5 18.7

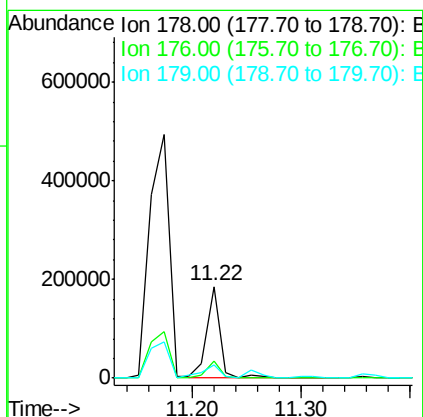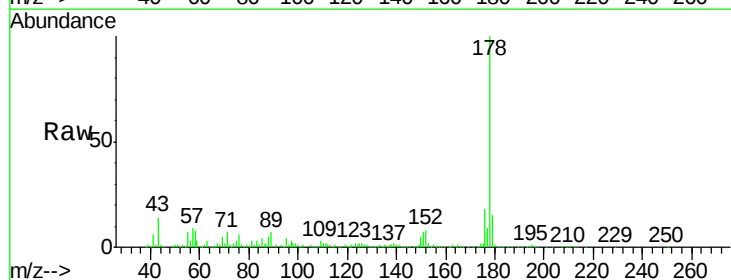



#72

Carbazole

Concen: 2.78 ng

RT: 11.38 min Scan# 813

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:167 Resp: 61654

Ion Ratio Lower Upper

167 100

166 22.4 17.6 26.4

139 14.8 11.8 17.8




Abundance Ion 167.00 (166.70 to 167.70): E


Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

Time-->

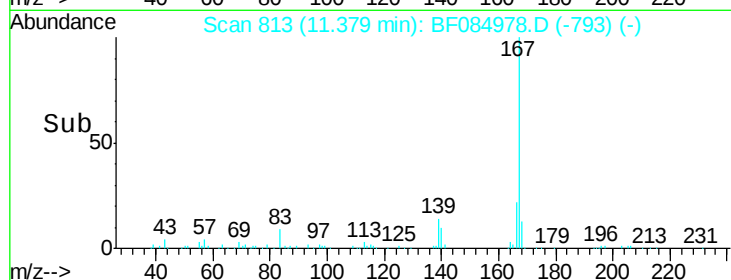

Time-->

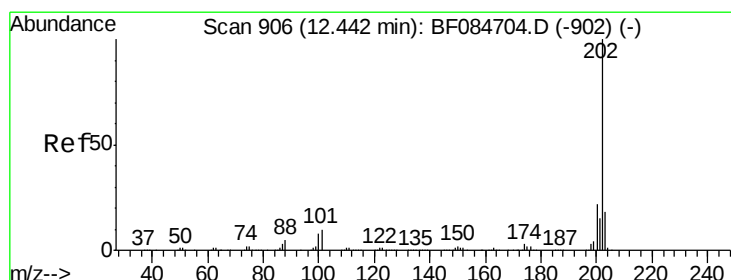

#74

Fluoranthene

Concen: 23.86 ng

RT: 12.35 min Scan# 898

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:202 Resp: 610511

Ion Ratio Lower Upper

202 100

101 11.2 0.0 32.8

203 18.2 0.0 37.9

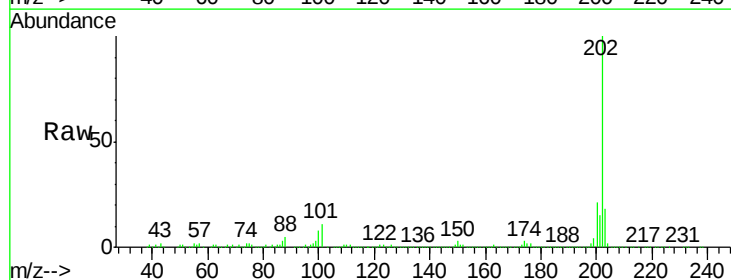


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

Time-->



Time-->



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.77 min Scan# 1022

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:240 Resp: 307456

Ion Ratio Lower Upper

240 100

120 16.1 9.5 14.3#




236 25.8 20.6 31.0

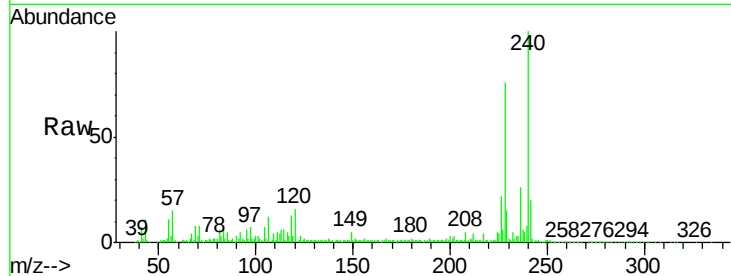

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

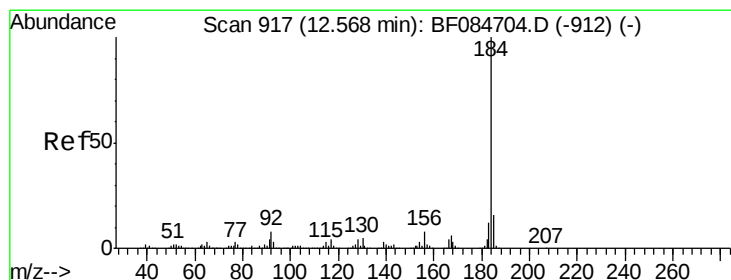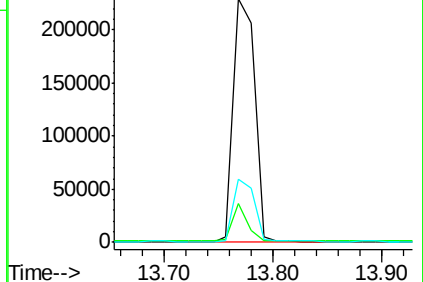

#76

Benzidine

Concen: 6.93 ng

RT: 12.51 min Scan# 912

Delta R.T. -0.03 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:184 Resp: 593

Ion Ratio Lower Upper

184 100

185 126.2 12.2 18.2#



183 126.8 9.8 14.8#




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

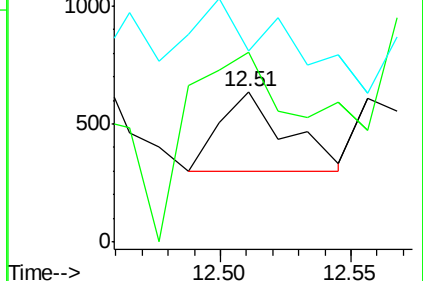



#77

Pyrene

Concen: 23.11 ng

RT: 12.58 min Scan# 918

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:202 Resp: 543976

Ion Ratio Lower Upper

202 100

200 20.6 17.2 25.8




203 18.0 14.3 21.5

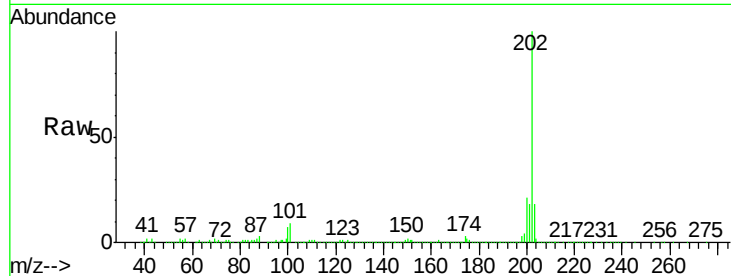

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

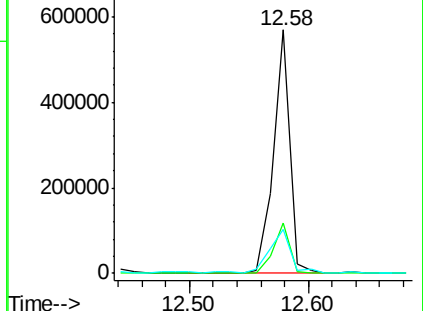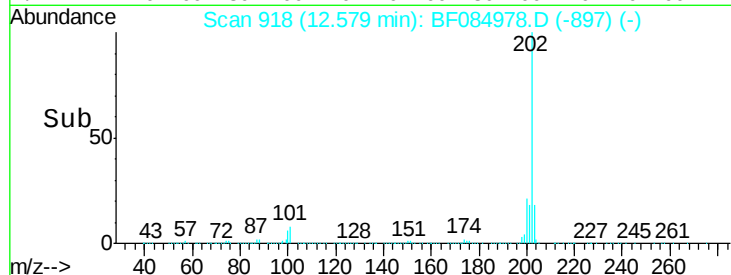

#78

Terphenyl-d14

Concen: 69.09 ng

RT: 12.73 min Scan# 931

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:244 Resp: 937434

Ion Ratio Lower Upper

244 100

212 7.6 5.7 8.5



122 14.6 7.4 11.0#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

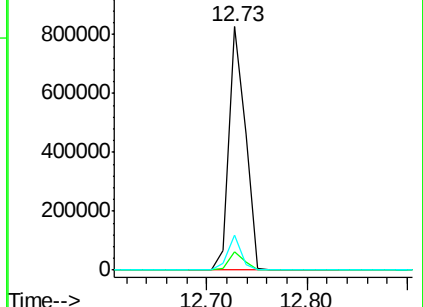



#80

Benzo(a)anthracene

Concen: 12.37 ng

RT: 13.77 min Scan# 1022

Delta R.T. -0.06 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:228 Resp: 235969

Ion Ratio Lower Upper

228 100

226 28.7 21.8 32.6




229 20.0 15.8 23.8

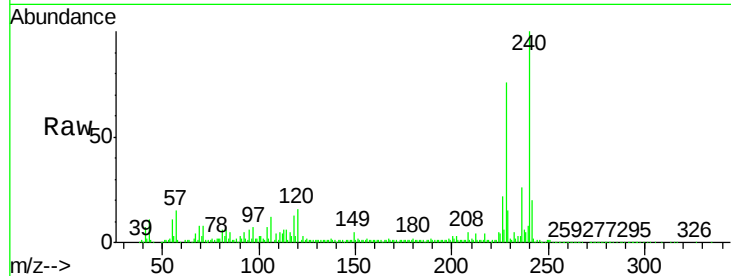

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

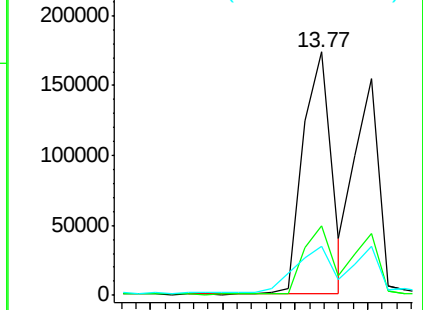

#82

Chrysene

Concen: 12.75 ng

RT: 13.77 min Scan# 1022

Delta R.T. -0.09 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:228 Resp: 235969

Ion Ratio Lower Upper

228 100

226 28.7 24.3 36.5



229 20.0 16.1 24.1




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

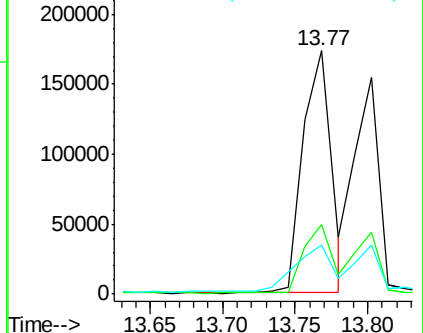


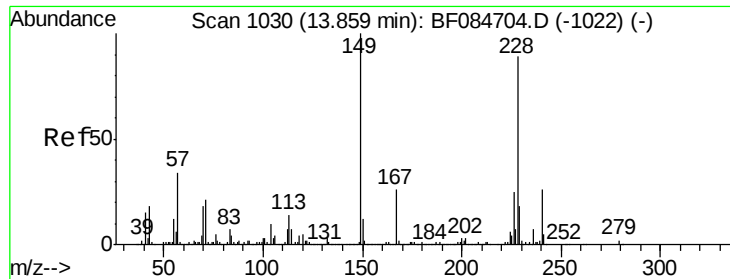




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 2.35 ng
 RT: 13.78 min Scan# 1023
 Delta R.T. -0.06 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)

Tgt Ion:149 Resp: 31258
 Ion Ratio Lower Upper
 149 100
 167 32.9 19.7 29.5#
 279 5.8 1.8 2.6#

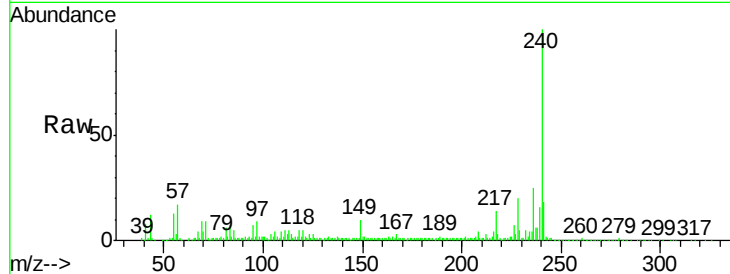


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

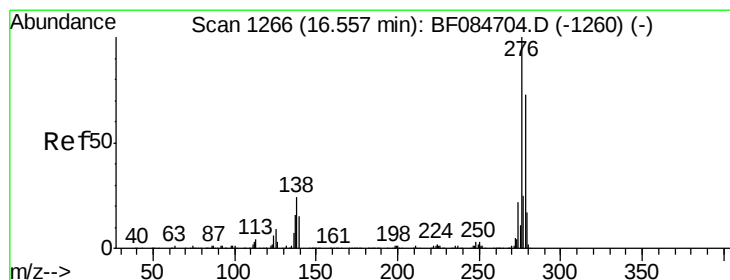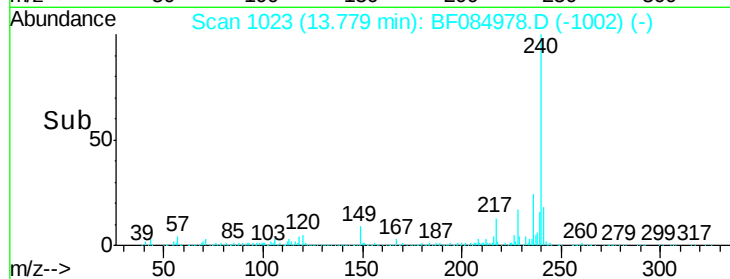
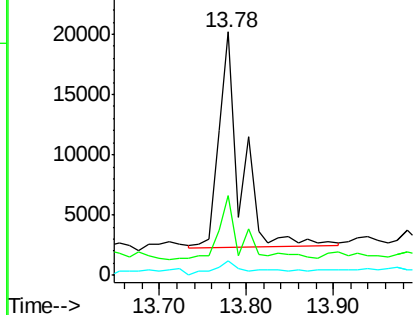



#85
 Indeno(1,2,3-cd)pyrene
 Concen: 6.56 ng
 RT: 16.40 min Scan# 1252
 Delta R.T. -0.10 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Tgt Ion:276 Resp: 95549
 Ion Ratio Lower Upper
 276 100
 138 21.8 20.6 30.8
 277 21.3 20.1 30.1

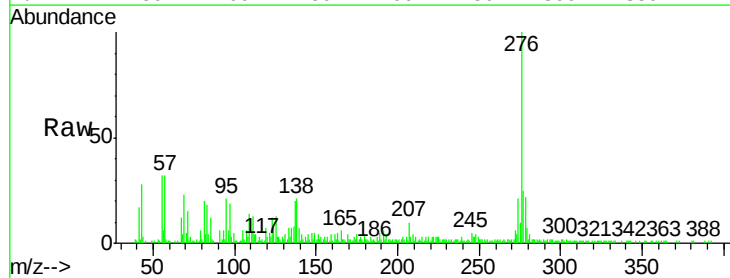

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

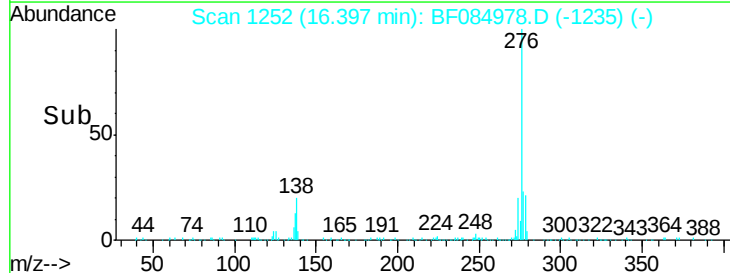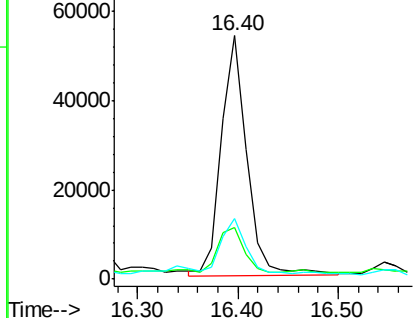







#86
Perylene-d12
Concen: 20.00 ng
RT: 15.14 min Scan# 1142
Delta R.T. -0.07 min
Lab File: BF084978.D
Acq: 10 Feb 2016 3:22

Instrument :
BNA_F
ClientSampleId :
S4-B005(0-2)

Tgt Ion:	264	Resp:	286203
Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.4	29.2
265	23.0	17.8	26.6

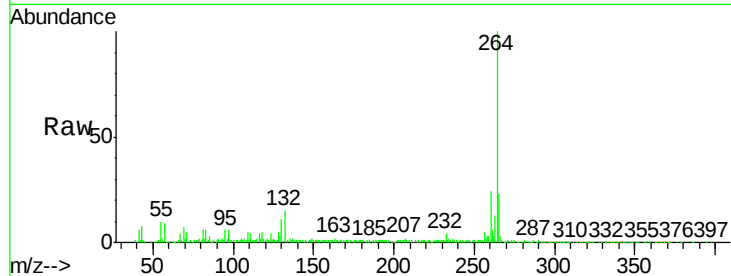


Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E


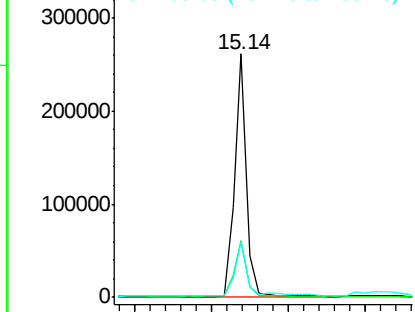



#87
Benzo(b)fluoranthene
Concen: 15.91 ng
RT: 14.77 min Scan# 1110
Delta R.T. -0.06 min
Lab File: BF084978.D
Acq: 10 Feb 2016 3:22

Tgt Ion:	252	Resp:	305904
Ion	Ratio	Lower	Upper
252	100		
253	23.8	17.3	25.9
125	13.4	6.5	9.7#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

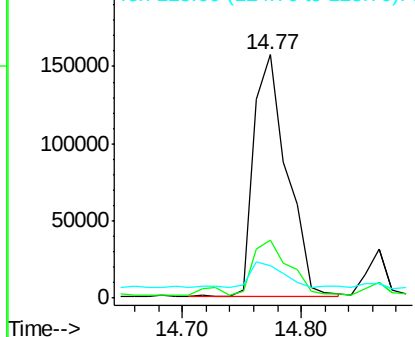



#88

Benzo(k)fluoranthene

Concen: 19.24 ng

RT: 14.77 min Scan# 1110

Delta R.T. -0.08 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22

Instrument :

BNA_F

ClientSampleId :

S4-B005(0-2)


Tgt Ion:252 Resp: 305904

Ion Ratio Lower Upper

252 100

253 23.8 18.1 27.1




125 13.4 9.0 13.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

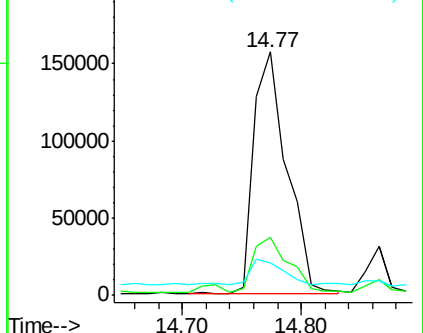

#89

Benzo(a)pyrene

Concen: 10.08 ng

RT: 15.08 min Scan# 1137

Delta R.T. -0.07 min

Lab File: BF084978.D

Acq: 10 Feb 2016 3:22


Tgt Ion:252 Resp: 165130

Ion Ratio Lower Upper

252 100

253 25.0 17.3 25.9



125 14.5 7.0 10.4#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

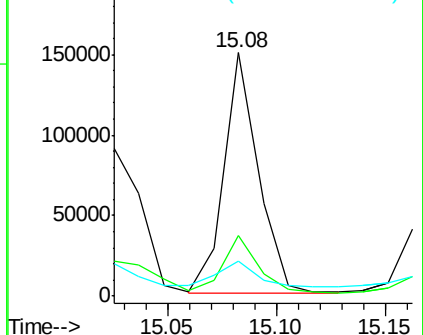



#91
 Benzo(g,h,i)perylene
 Concen: 6.37 ng
 RT: 16.77 min Scan# 1285
 Delta R.T. -0.11 min
 Lab File: BF084978.D
 Acq: 10 Feb 2016 3:22

Instrument :
 BNA_F
 ClientSampleId :
 S4-B005(0-2)

Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.3	18.8	28.2
138	20.7	17.8	26.6

