

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
 Data File : BF084980.D
 Acq On : 10 Feb 2016 4:18
 Operator : SJ/IZ
 Sample : H1361-06 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.750	231	233	242	rVB	262561	311526	24.76%	1.754%
2	5.207	271	273	276	rBV	1007729	1121088	89.10%	6.312%
3	6.282	364	367	369	rBV	1371701	1209189	96.10%	6.808%
4	6.396	375	377	380	rBV	1396230	1169850	92.98%	6.587%
5	6.636	395	398	400	rBV	801657	967520	76.90%	5.447%
6	6.785	409	411	414	rBV	1030053	891122	70.83%	5.017%
7	7.196	445	447	450	rBV	641984	667159	53.03%	3.756%
8	7.916	508	510	513	rBV	1136895	1230051	97.76%	6.926%
9	9.002	602	605	607	rBV	1083146	1150021	91.40%	6.475%
10	9.093	609	613	615	rVB	15988	18884	1.50%	0.106%
11	9.402	638	640	642	rBV	147519	150984	12.00%	0.850%
12	9.528	649	651	653	rBV	15680	15150	1.20%	0.085%
13	9.619	656	659	661	rVV	48739	45414	3.61%	0.256%
14	9.665	661	663	665	rVV	1262116	1216451	96.68%	6.849%
15	9.699	665	666	668	rVB	40570	30989	2.46%	0.174%
16	9.871	677	681	683	rBV2	22994	29278	2.33%	0.165%
17	10.076	696	699	700	rBV3	8355	14856	1.18%	0.084%
18	10.111	700	702	704	rVV	47316	51008	4.05%	0.287%
19	10.213	709	711	713	rVV	30782	26742	2.13%	0.151%
20	10.282	714	717	719	rBV4	8190	19260	1.53%	0.108%
21	10.328	719	721	724	rVV2	21229	33647	2.67%	0.189%
22	10.453	730	732	734	rBV	651554	609821	48.47%	3.433%
23	10.591	741	744	747	rBV2	48525	89479	7.11%	0.504%
24	10.682	747	752	753	rBV5	8460	21163	1.68%	0.119%
25	10.762	756	759	760	rBV3	11938	21460	1.71%	0.121%
26	11.002	778	780	781	rBV	13032	17118	1.36%	0.096%
27	11.036	781	783	787	rVB	43345	73387	5.83%	0.413%
28	11.139	790	792	796	rBV	830941	1252801	99.57%	7.054%
29	11.219	796	799	801	rBV	91983	86387	6.87%	0.486%
30	11.254	801	802	804	rBV	17105	17803	1.41%	0.100%
31	11.379	812	813	814	rBV	31405	26248	2.09%	0.148%
32	11.459	817	820	825	rVV4	16829	50441	4.01%	0.284%
33	11.642	834	836	837	rBV	48104	49101	3.90%	0.276%
34	11.676	837	839	841	rVV	58055	65248	5.19%	0.367%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
Data File : BF084980.D
Acq On : 10 Feb 2016 4:18
Operator : SJ/IZ
Sample : H1361-06 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.722	841	843	844	rVV	30489	28801	2.29%	0.162%
36	11.756	844	846	850	rVB2	71830	115144	9.15%	0.648%
37	11.939	861	862	863	rBV	29861	24387	1.94%	0.137%
38	12.191	882	884	885	rBV	37701	42583	3.38%	0.240%
39	12.282	890	892	893	rVB	20646	24585	1.95%	0.138%
40	12.351	896	898	900	rBV	418828	375493	29.84%	2.114%
41	12.408	900	903	905	rBV4	14750	30782	2.45%	0.173%
42	12.579	915	918	919	rBV	288006	403673	32.08%	2.273%
43	12.625	919	922	925	rVB4	38771	81156	6.45%	0.457%
44	12.728	929	931	933	rVV	946568	828933	65.88%	4.667%
45	12.797	933	937	941	rVV3	25979	47874	3.80%	0.270%
46	12.968	950	952	954	rBV2	36100	51299	4.08%	0.289%
47	13.002	954	955	957	rBV	34616	52881	4.20%	0.298%
48	13.402	988	990	992	rBV2	63535	107014	8.51%	0.603%
49	13.517	998	1000	1001	rBV2	32009	40772	3.24%	0.230%
50	13.768	1019	1022	1027	rBV2	834979	1258196	100.00%	7.084%
51	14.762	1107	1109	1113	rBV	140238	292230	23.23%	1.645%
52	15.025	1130	1132	1135	rVB	91855	116144	9.23%	0.654%
53	15.082	1135	1137	1139	rBV	131057	156291	12.42%	0.880%
54	15.140	1139	1142	1144	rBV	595118	712107	56.60%	4.009%
55	16.385	1249	1251	1255	rVB2	60556	124277	9.88%	0.700%
56	16.763	1282	1284	1290	rVB	49672	95746	7.61%	0.539%


Sum of corrected areas: 17761014

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
Data File : BF084980.D
Acq On : 10 Feb 2016 4:18
Operator : SJ/IZ
Sample : H1361-06 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
WC-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

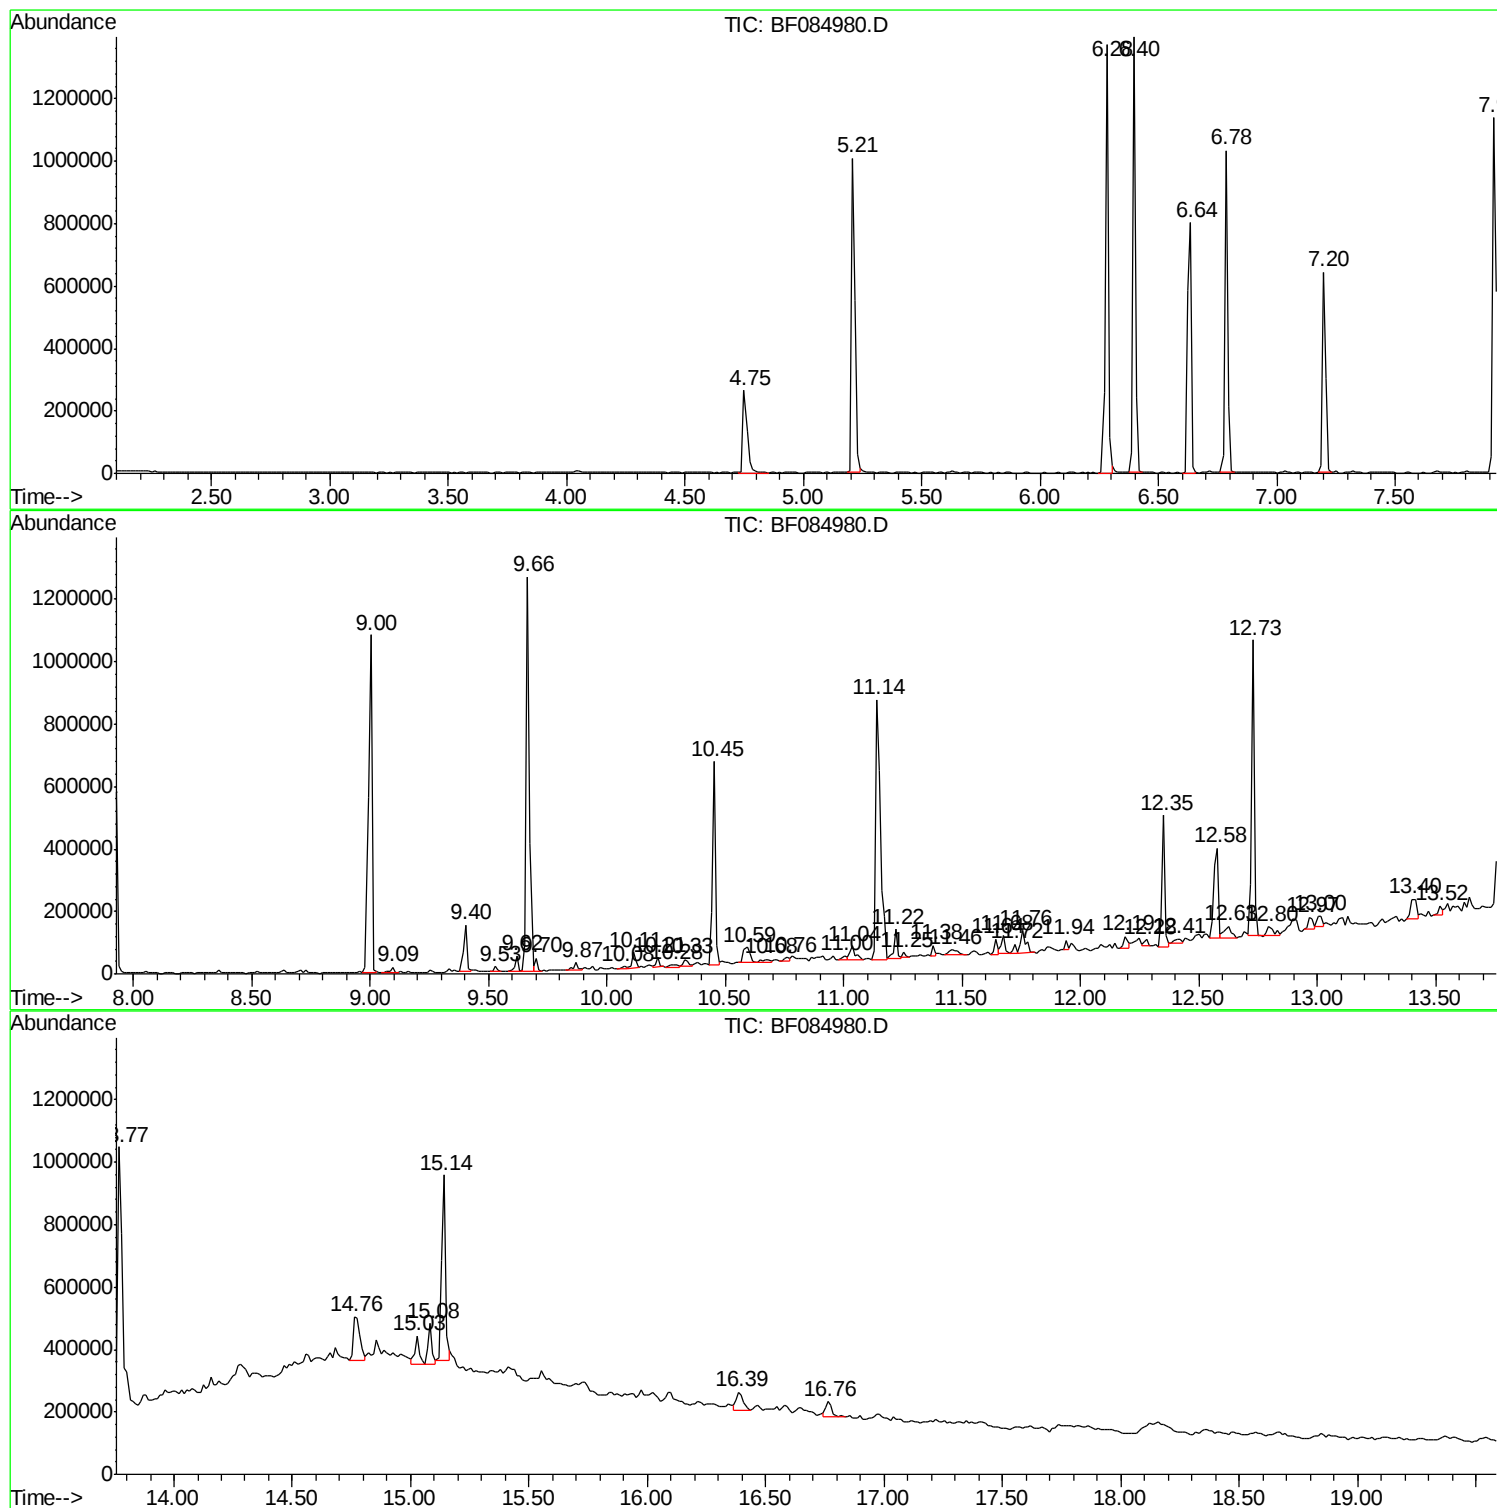

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020916\
Data File : BF084980.D
Acq On : 10 Feb 2016 4:18
Operator : SJ/IZ
Sample : H1361-06 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.75	6.44 ng	311526	1,4-Dichlorobenzene-d4	6.64

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
4			3-Hexanol	102	C6H14O	000623-37-0	33
5			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33

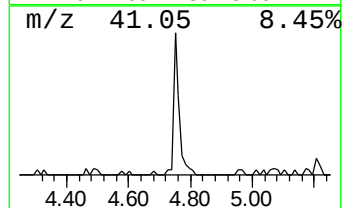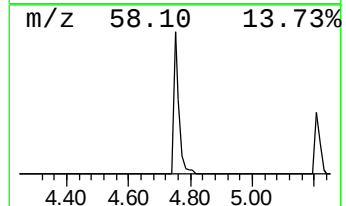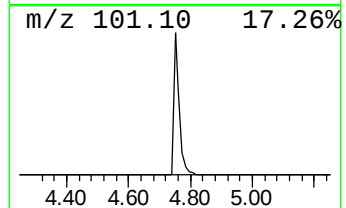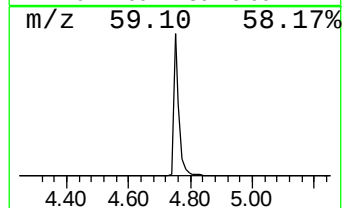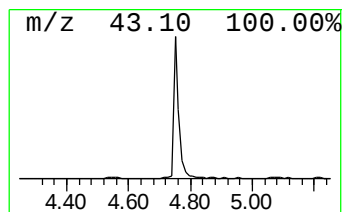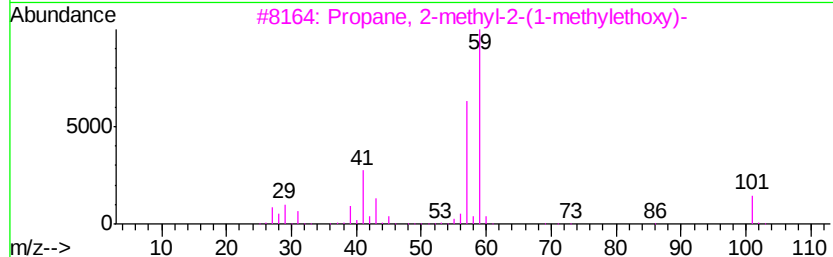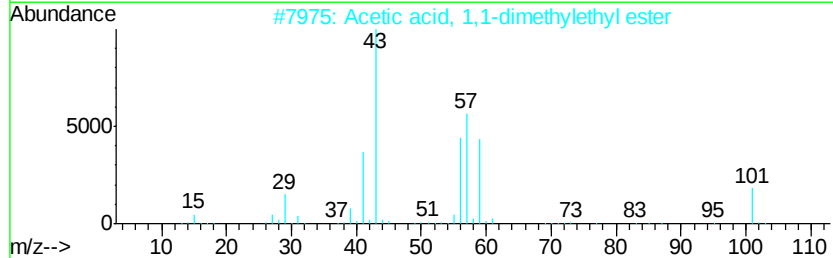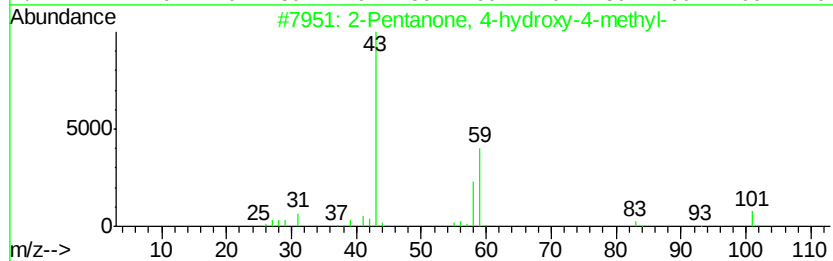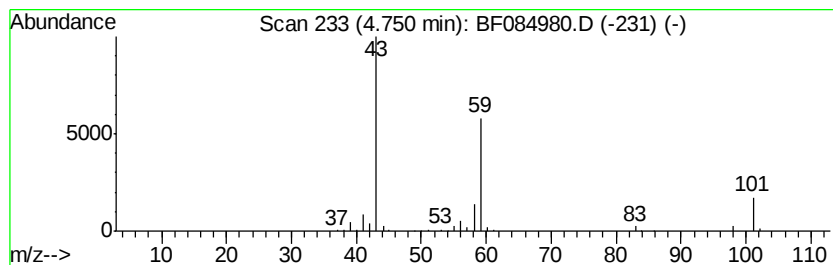

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
Data File : BF084980.D
Acq On : 10 Feb 2016 4:18
Operator : SJ/IZ
Sample : H1361-06 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.75	6.4	ng	311526	1	6.64	967520	20.0