


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
 Data File : BF084943.D
 Acq On : 9 Feb 2016 11:07
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 13:28:51 2016

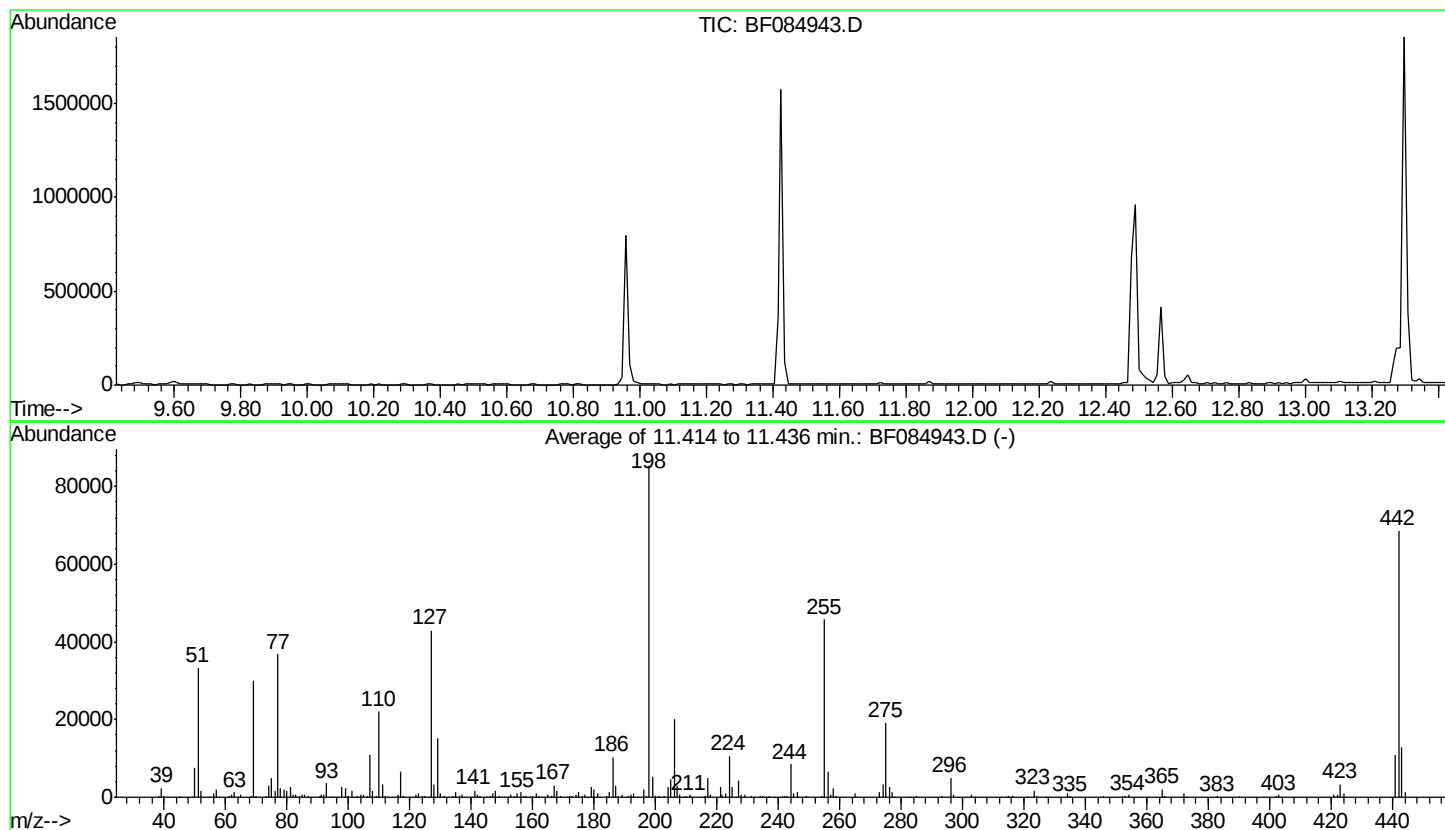

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	33447	PASS
68	69	0.00	2	1.5	444	PASS
69	198	0.00	100	35.2	30063	PASS
70	69	0.00	2	0.8	248	PASS
127	198	10	80	50.4	42986	PASS
197	198	0.00	2	0.5	465	PASS
198	198	100	100	100.0	85357	PASS
199	198	5	9	6.4	5436	PASS
275	198	10	60	22.5	19214	PASS
365	198	1	100	2.4	2048	PASS
441	442	0.01	24	16.0	10976	PASS
442	198	50	100	80.4	68610	PASS
443	442	15	24	19.0	13018	PASS