


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF020916\
 Data File : BF084962.D
 Acq On : 9 Feb 2016 19:57
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 13:28:51 2016

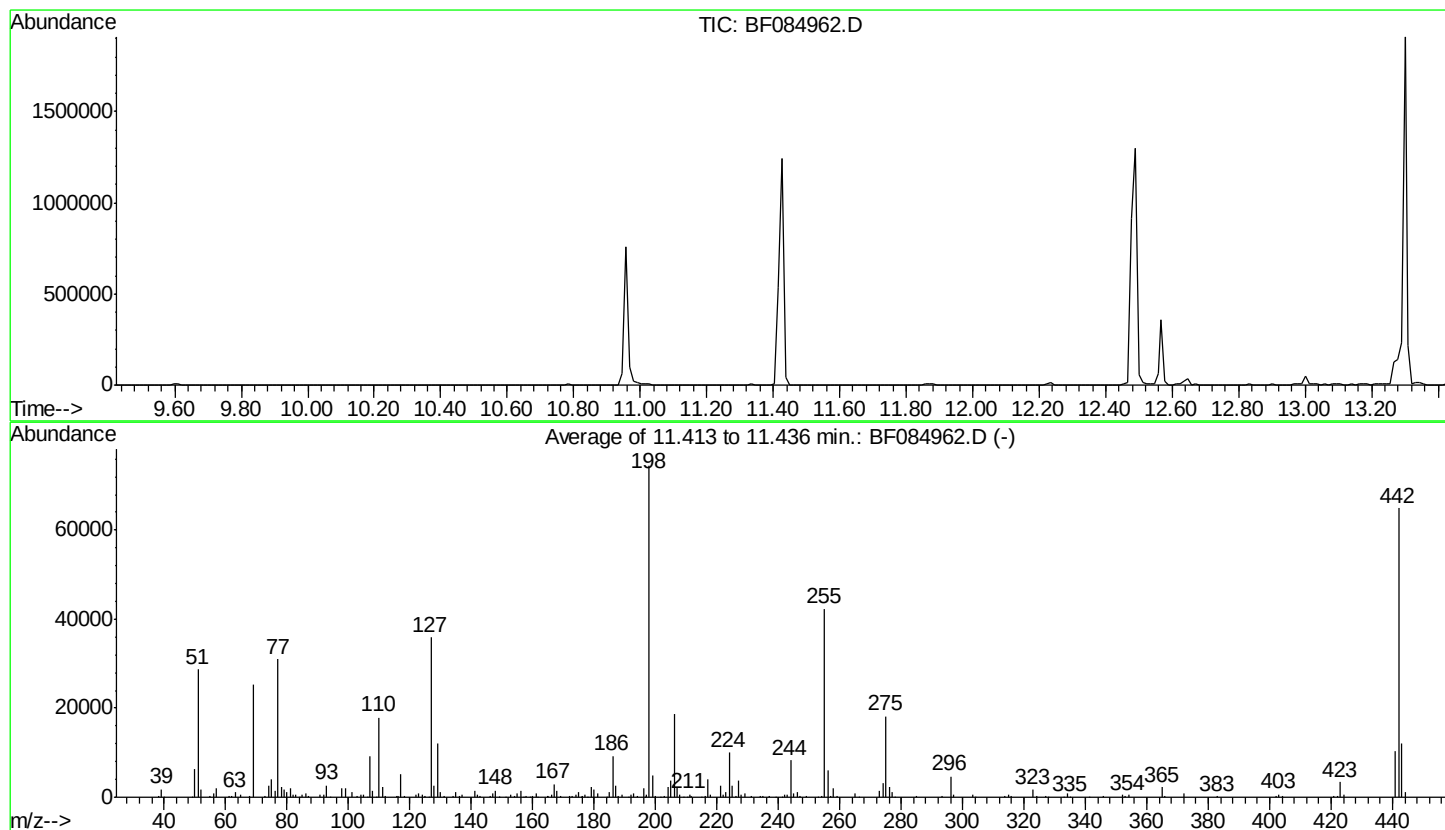

AutoFind: Scans 816, 817, 818; Background Corrected with Scan 812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	28646	PASS
68	69	0.00	2	1.7	429	PASS
69	198	0.00	100	34.2	25458	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	35920	PASS
197	198	0.00	2	0.6	450	PASS
198	198	100	100	100.0	74491	PASS
199	198	5	9	6.6	4901	PASS
275	198	10	60	24.3	18131	PASS
365	198	1	100	3.0	2260	PASS
441	442	0.01	24	15.8	10283	PASS
442	198	50	100	87.2	64935	PASS
443	442	15	24	18.6	12078	PASS