
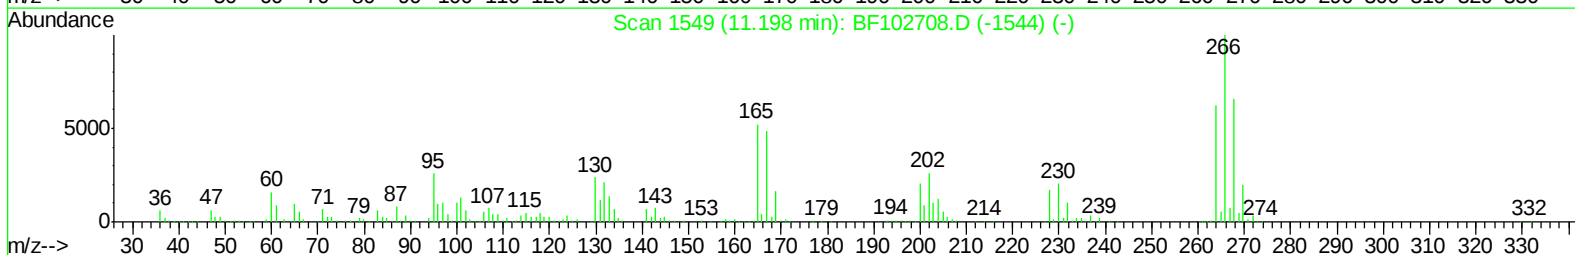
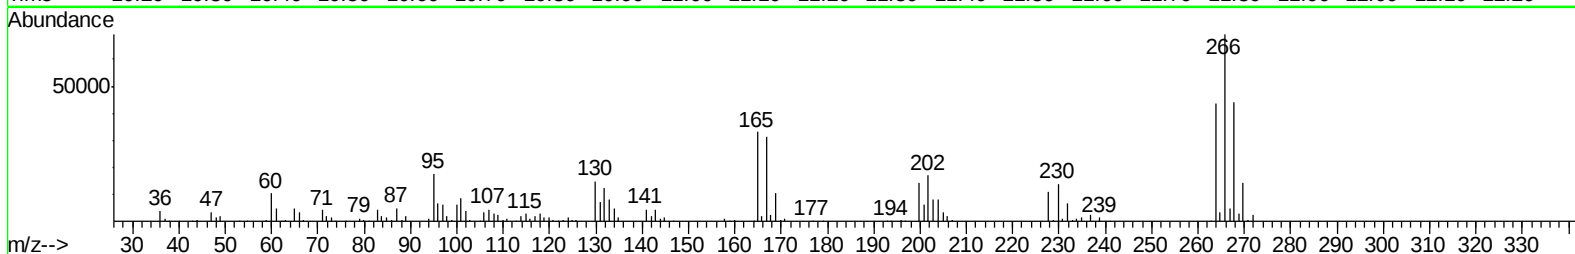


Data Path : Z:\HPCHEM1\BNA F\DATA\BF020918\
Data File : BF102902.D
Acq On : 9 Feb 2018 22:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 02:07:32 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 12:44:16 2018
Response via : Initial Calibration

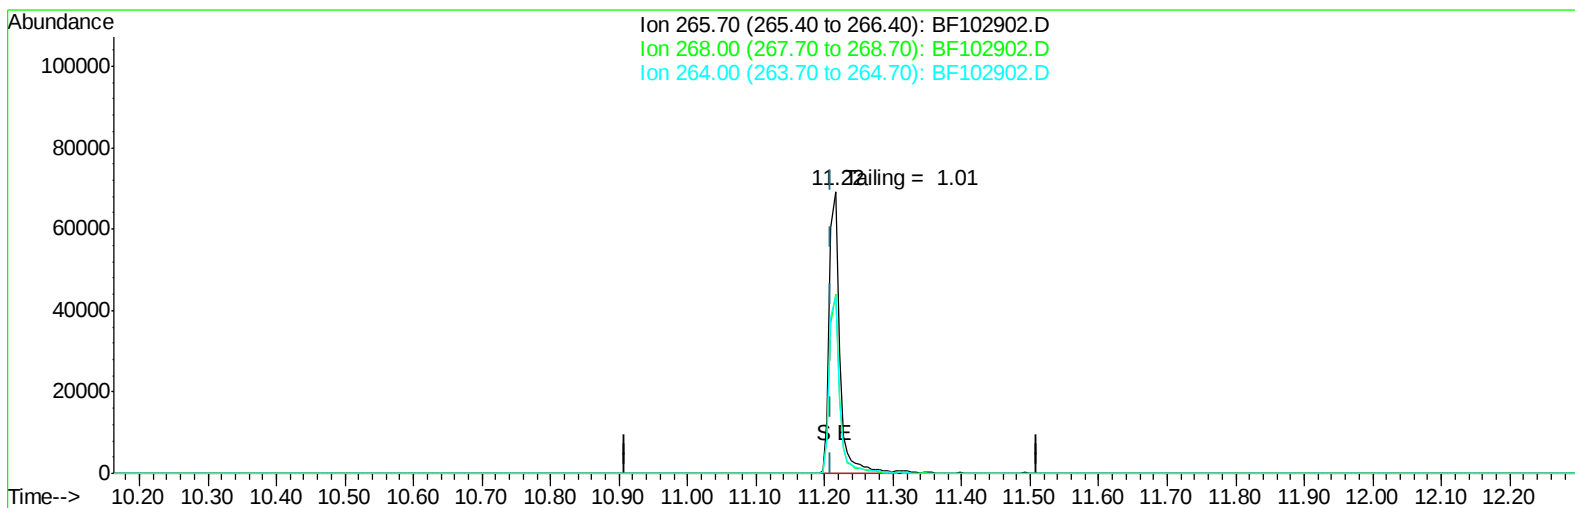

TIC: BF102902.D

(69) Pentachlorophenol (C)




11.216min (+0.006) 59779.50ng

response 71664

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.66
264.00	61.90	62.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF020918\
 Data File : BF102902.D
 Acq On : 9 Feb 2018 22:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 02:07:32 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 12:44:16 2018
 Response via : Initial Calibration

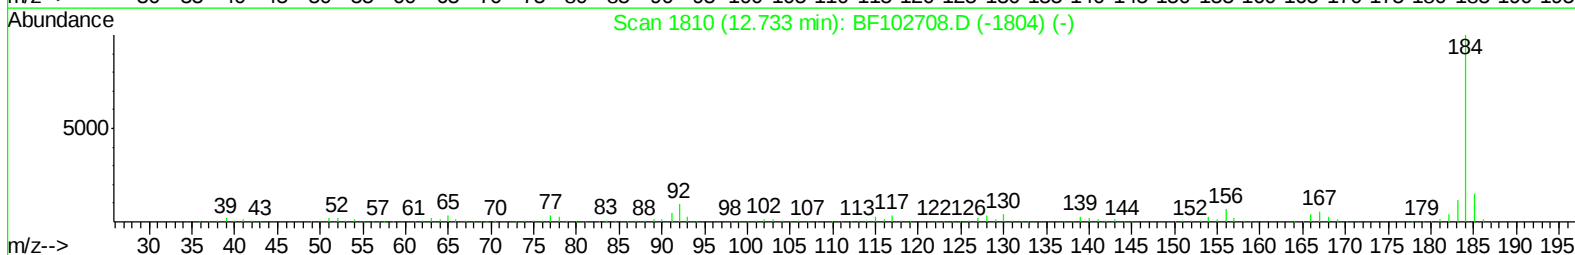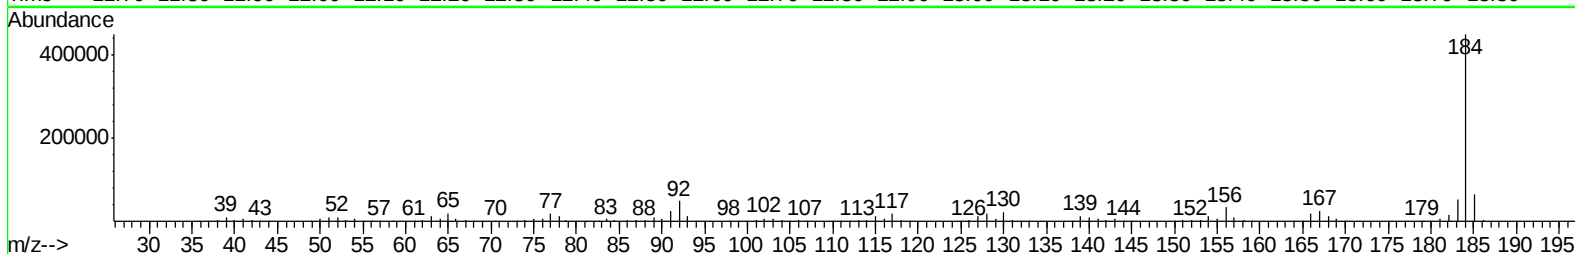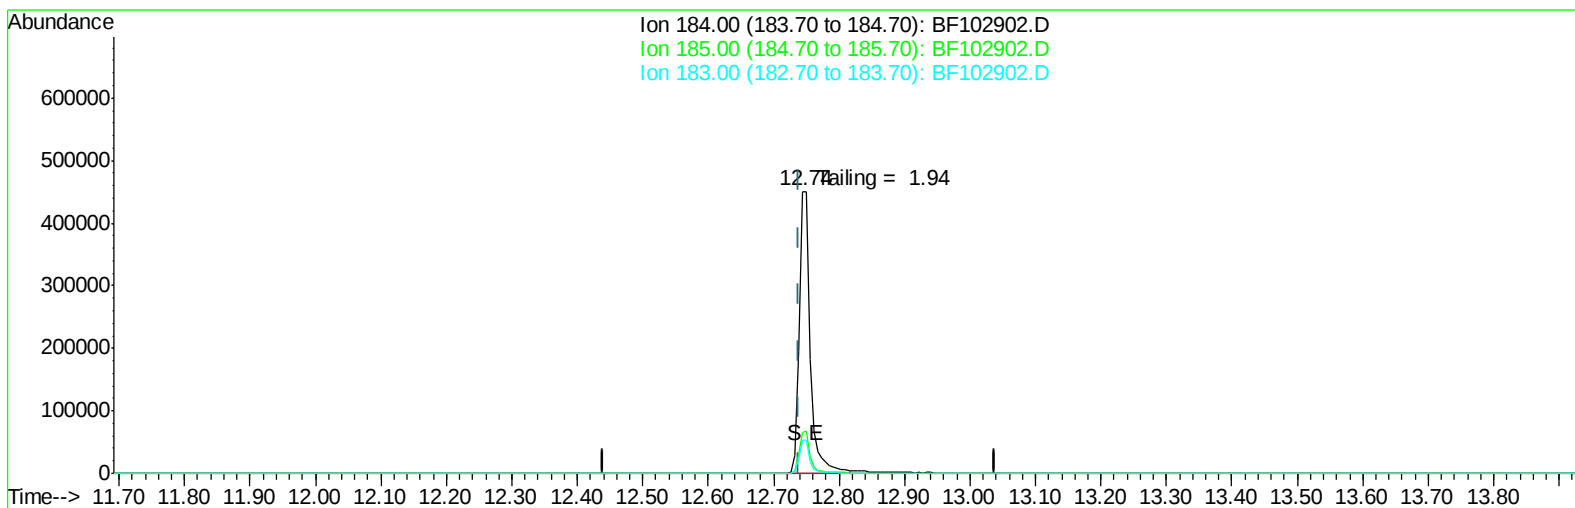

TIC: BF102902.D

(76) Benzidine

12.745min (+0.006) 32270.53ng

response 544320

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.78
183.00	11.60	11.76
0.00	0.00	0.00