


Data Path : Z:\HPCHEM1\BNA F\Data\BF020918\
 Data File : BF102875.D
 Acq On : 9 Feb 2018 9:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 05 12:44:16 2018

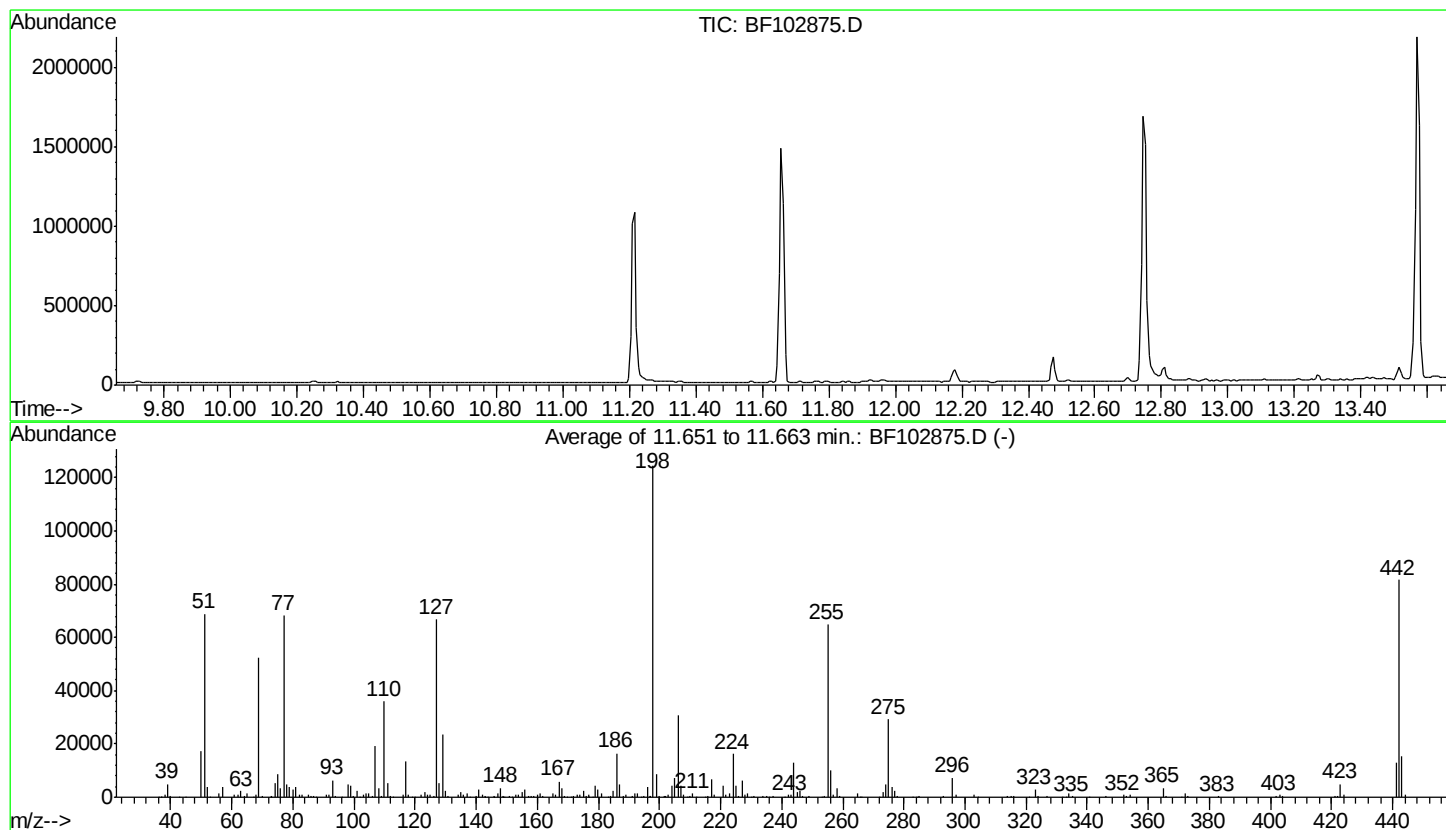

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	68879	PASS
68	69	0.00	2	1.8	968	PASS
69	198	0.00	100	42.1	52362	PASS
70	69	0.00	2	0.8	422	PASS
127	198	10	80	53.6	66741	PASS
197	198	0.00	2	0.5	668	PASS
198	198	100	100	100.0	124482	PASS
199	198	5	9	6.9	8592	PASS
275	198	10	60	23.4	29101	PASS
365	198	1	100	2.8	3493	PASS
441	443	0.01	100	82.9	12875	PASS
442	198	50	100	65.4	81469	PASS
443	442	15	24	19.1	15530	PASS