


Data Path : Z:\HPCHEM1\BNA F\Data\BF020918\
Data File : BF102902.D
Acq On : 9 Feb 2018 22:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 05 12:44:16 2018

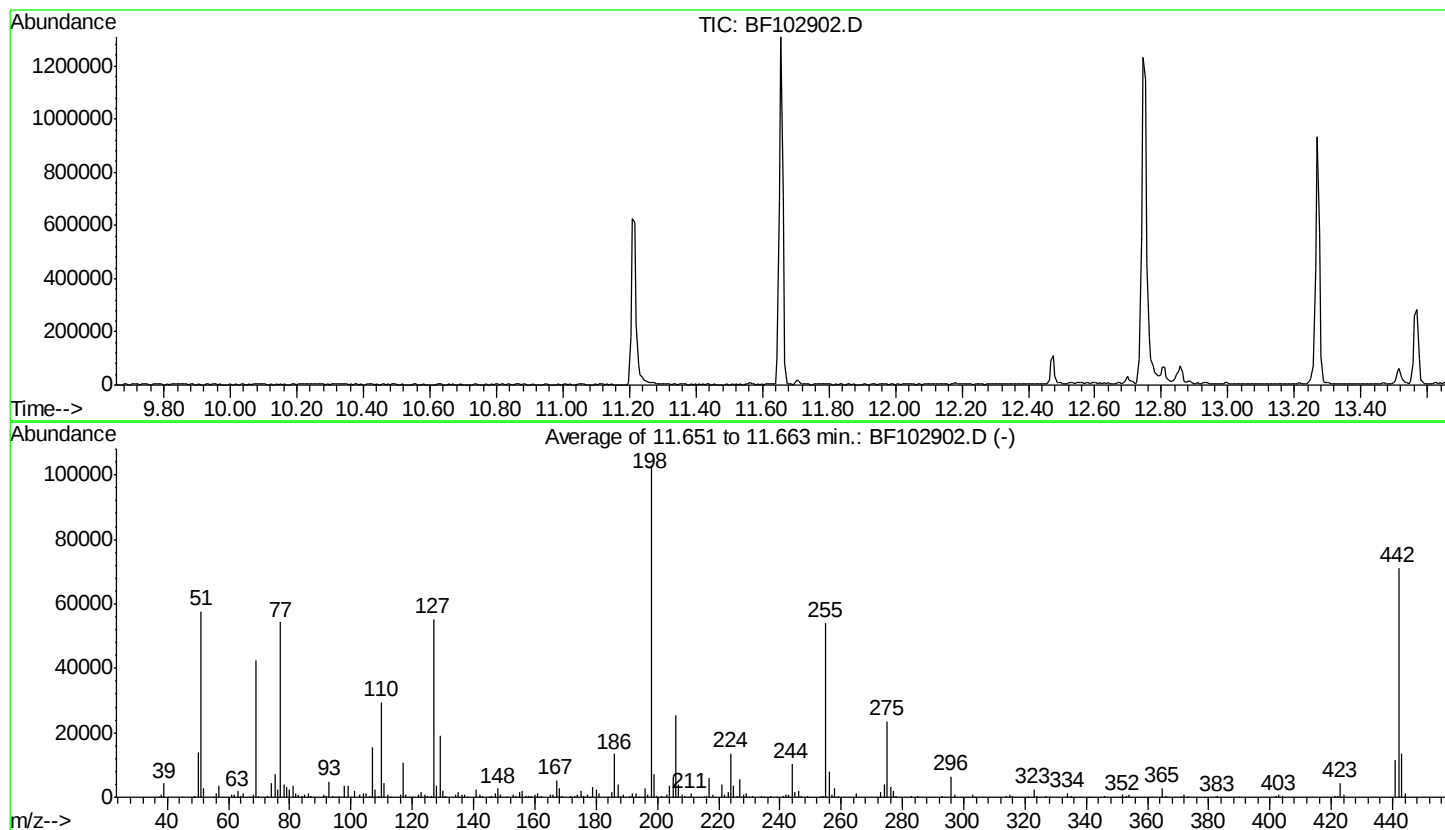

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.0	57629	PASS
68	69	0.00	2	1.8	759	PASS
69	198	0.00	100	41.4	42584	PASS
70	69	0.00	2	0.6	265	PASS
127	198	10	80	53.7	55226	PASS
197	198	0.00	2	0.9	884	PASS
198	198	100	100	100.0	102898	PASS
199	198	5	9	7.0	7194	PASS
275	198	10	60	22.8	23505	PASS
365	198	1	100	2.8	2883	PASS
441	443	0.01	100	87.5	11697	PASS
442	198	50	100	69.1	71114	PASS
443	442	15	24	18.8	13362	PASS