
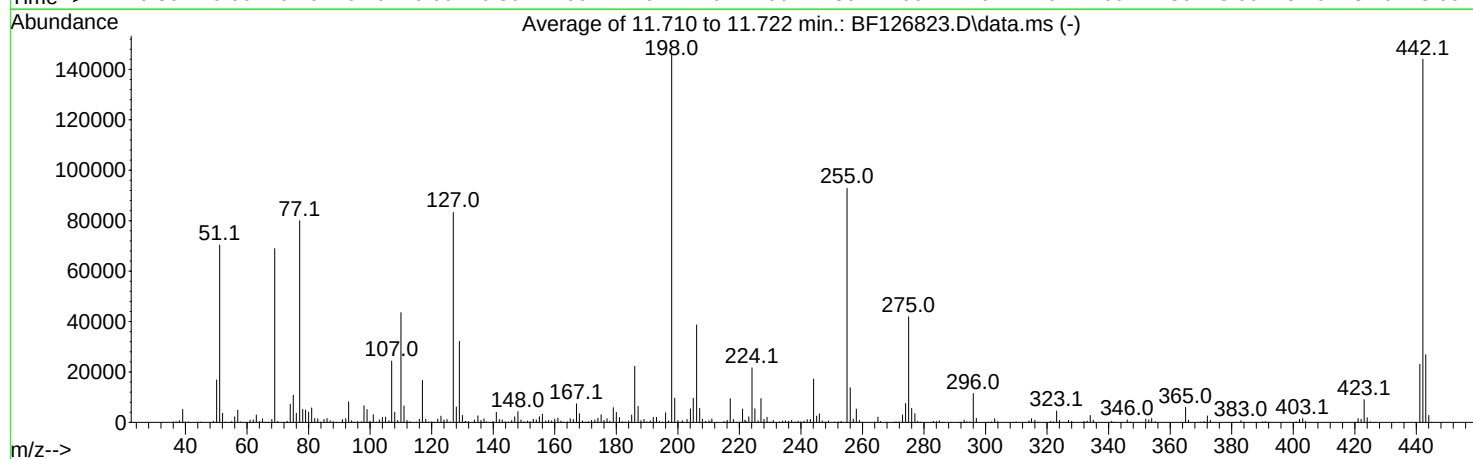


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020922\
 Data File : BF126823.D
 Acq On : 09 Feb 2022 13:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 10 00:44:00 2022

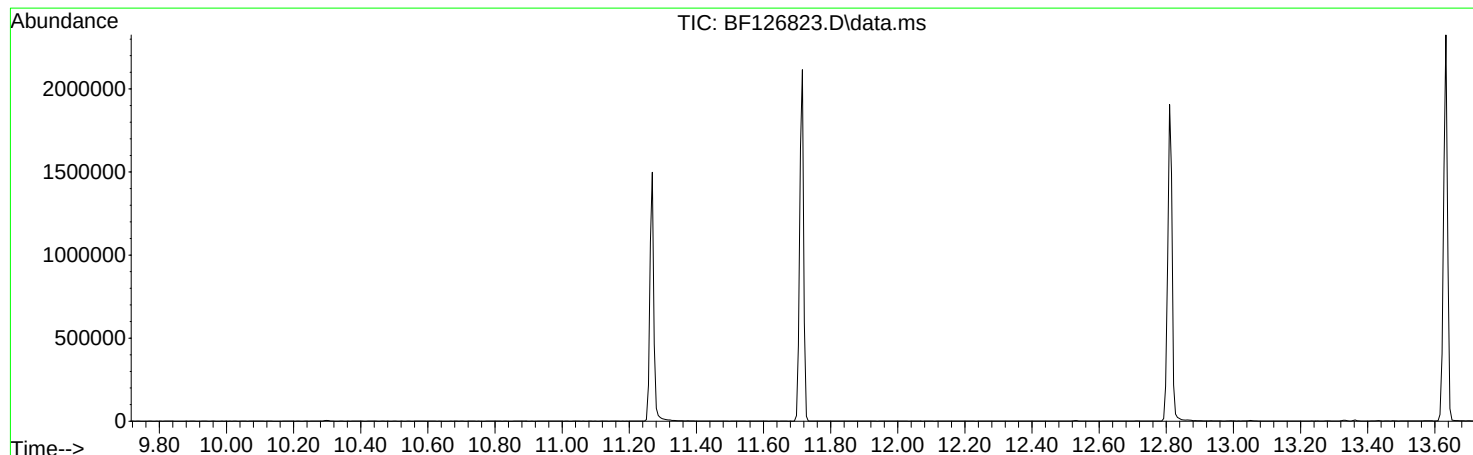




AutoFind: Scans 1466, 1467, 1468; Background Corrected with Scan 1461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	70333	PASS
68	69	0.00	2	1.8	1225	PASS
69	198	0.00	100	47.2	68937	PASS
70	69	0.00	2	0.6	414	PASS
127	198	10	80	57.1	83299	PASS
197	198	0.00	2	0.5	661	PASS
198	198	100	100	100.0	145925	PASS
199	198	5	9	6.6	9599	PASS
275	198	10	60	28.7	41923	PASS
365	198	1	100	4.1	5957	PASS
441	198	0.01	100	15.8	23054	PASS
442	442	50	100	100.0	144059	PASS
443	442	15	24	18.7	26872	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020922\
Data File : BF126823.D
Acq On : 09 Feb 2022 13:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 04:28:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

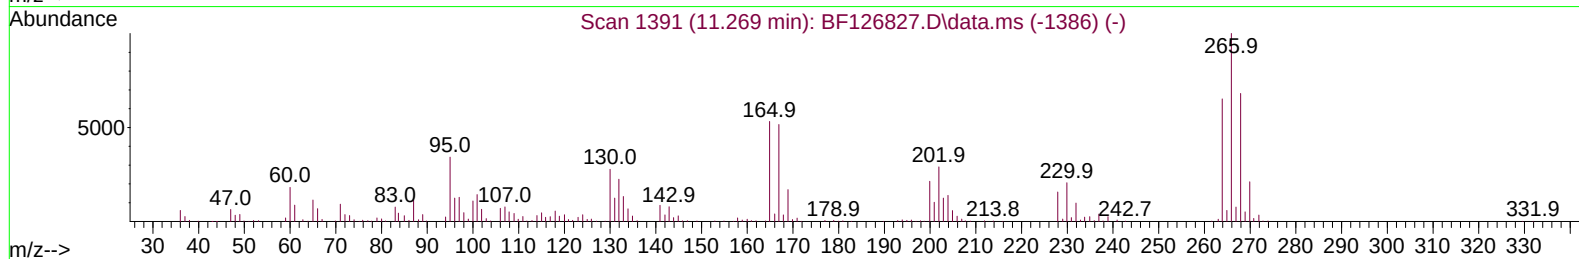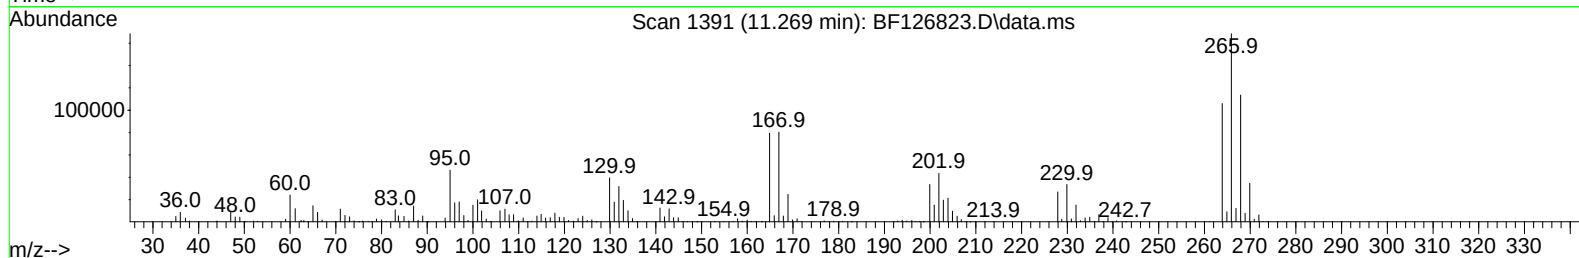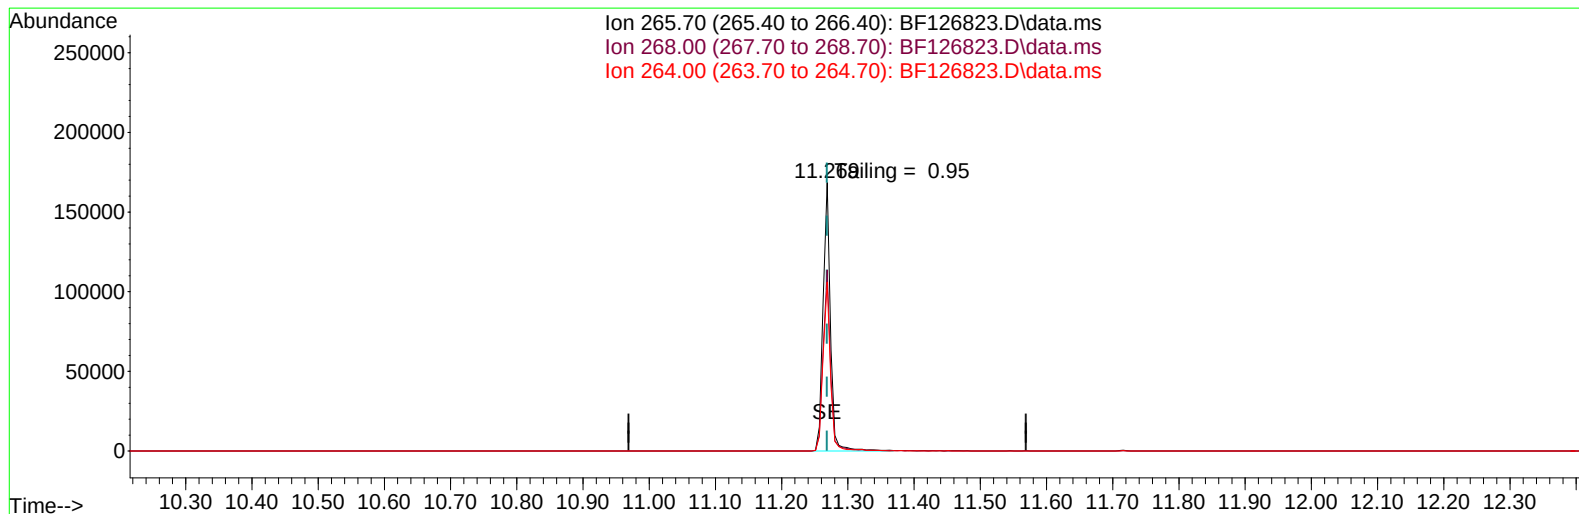

TIC: BF126823.D\data.ms

(70) Pentachlorophenol (C)

11.269min (+ 0.000) 23361.01 ng




response 131368

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	67.42
264.00	65.20	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020922\
Data File : BF126823.D
Acq On : 09 Feb 2022 13:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 04:28:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

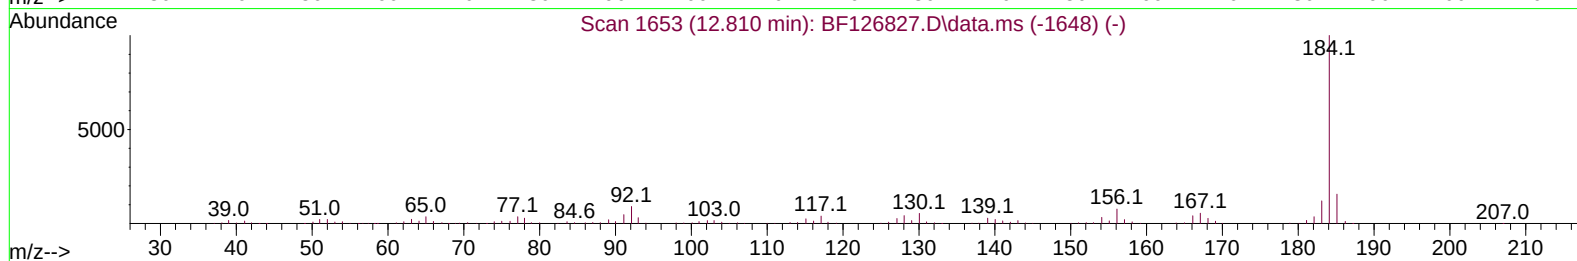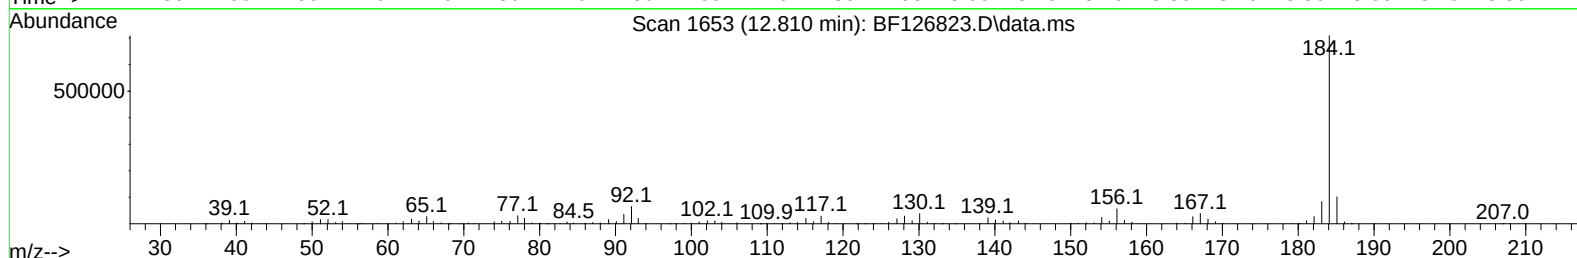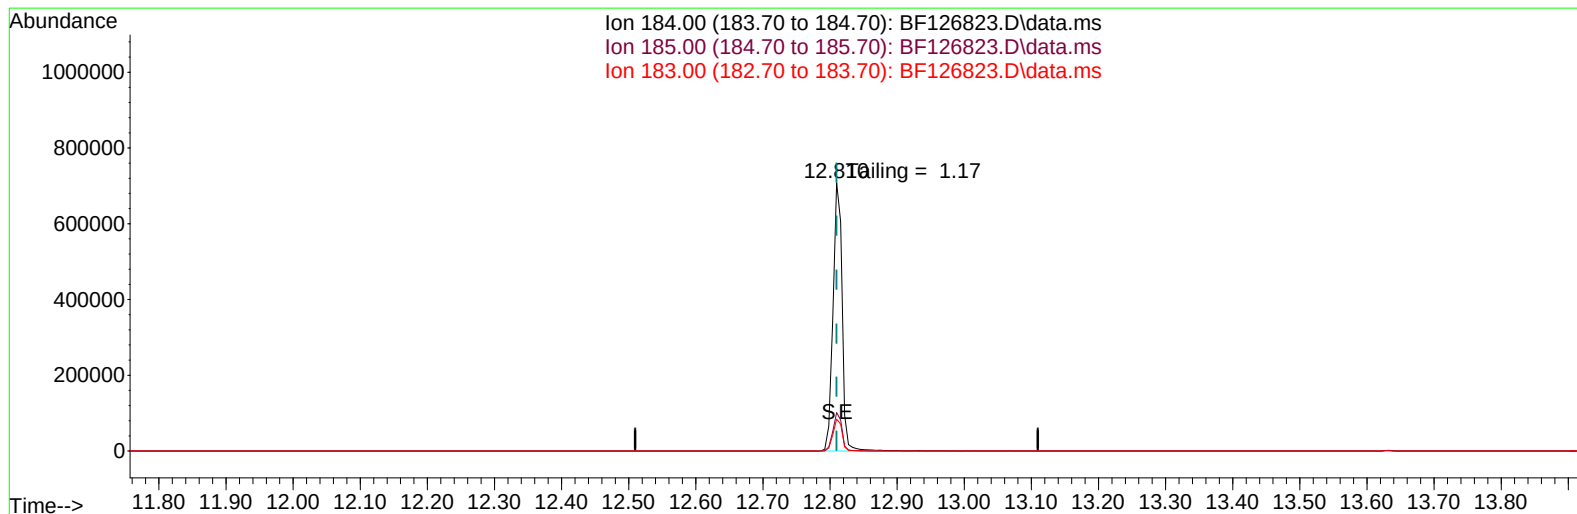

TIC: BF126823.D\data.ms

(77) Benzidine

12.810min (+ 0.000) 0.00 ng

response 663034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.30
183.00	12.00	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2022	BNA_F	<u>BF126823.D</u>
Compound Name	Response	Retention Time
DDT	323916	13.633
DDD	2612	13.363
DDE	280	12.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2892	326808	0.88

Instrument :
BNA_F
ClientSampleId :
DFTPP