


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020923\
Data File : BF132371.D
Acq On : 09 Feb 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 09 01:56:26 2023

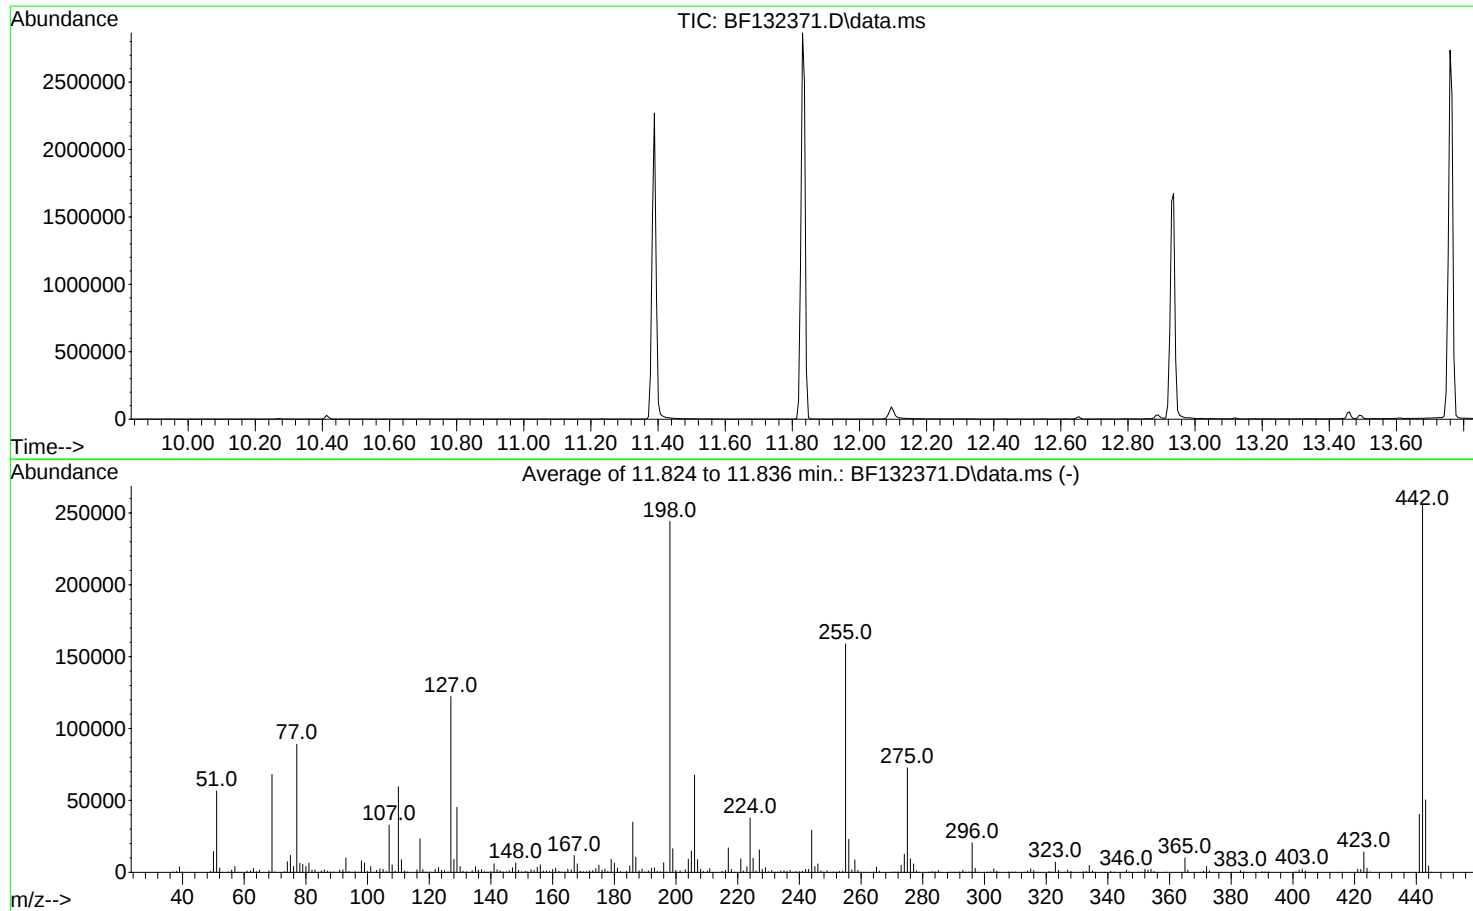




AutoFind: Scans 1528, 1529, 1530; Background Corrected with Scan 1523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	56629	PASS
68	69	0.00	2	1.5	1006	PASS
69	198	0.00	100	27.9	68213	PASS
70	69	0.00	2	0.6	441	PASS
127	198	10	80	50.1	122285	PASS
197	198	0.00	2	0.1	338	PASS
198	198	100	100	100.0	244245	PASS
199	198	5	9	6.7	16407	PASS
275	198	10	60	29.7	72659	PASS
365	198	1	100	4.1	9922	PASS
441	198	0.01	100	16.5	40331	PASS
442	442	50	100	100.0	255955	PASS
443	442	15	24	19.7	50409	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020923\
 Data File : BF132371.D
 Acq On : 09 Feb 2023 09:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 10 02:16:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 09 01:56:26 2023
 Response via : Initial Calibration

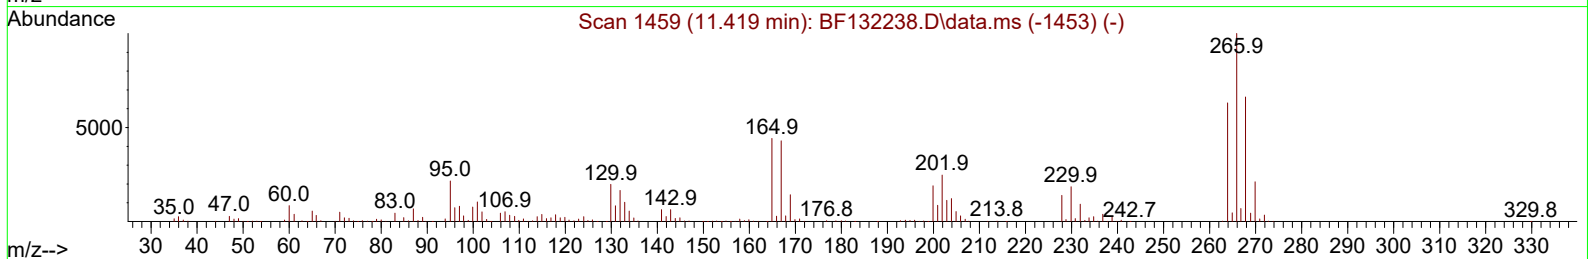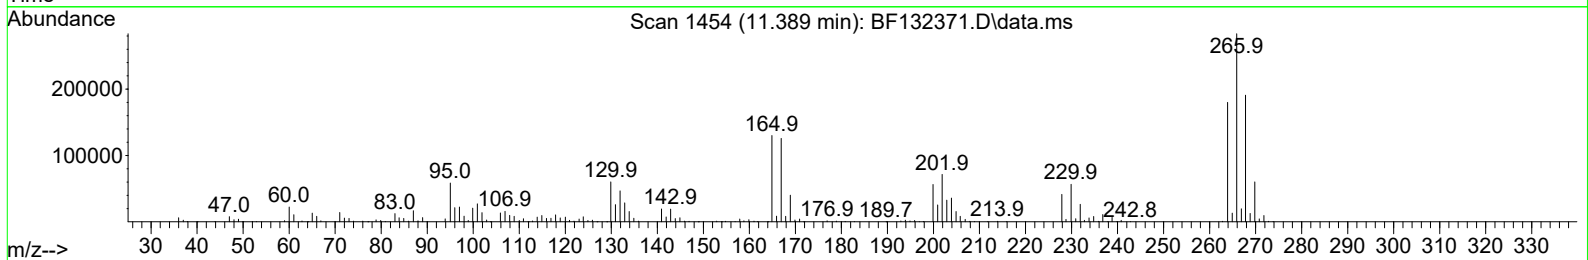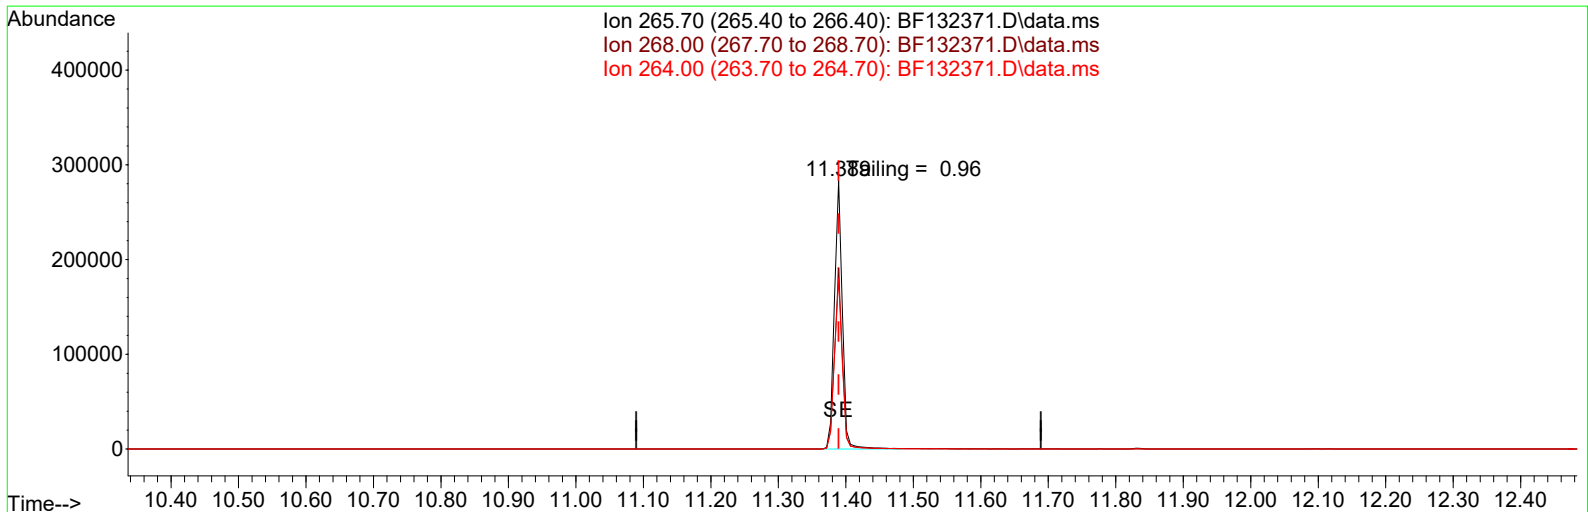

TIC: BF132371.D\data.ms

(70) Pentachlorophenol (C)

11.389min (0.000) 28141.69 ng




response 233214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	67.31
264.00	63.10	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF020923\
Data File : BF132371.D
Acq On : 09 Feb 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 10 02:16:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 09 01:56:26 2023
Response via : Initial Calibration

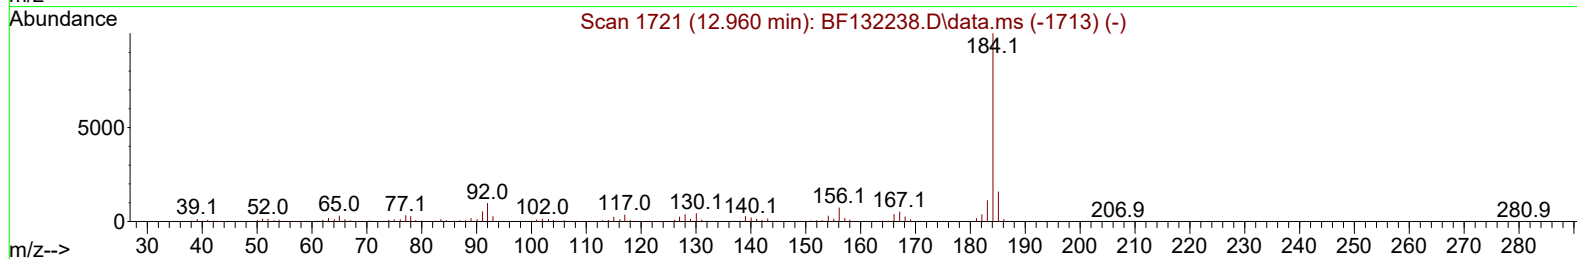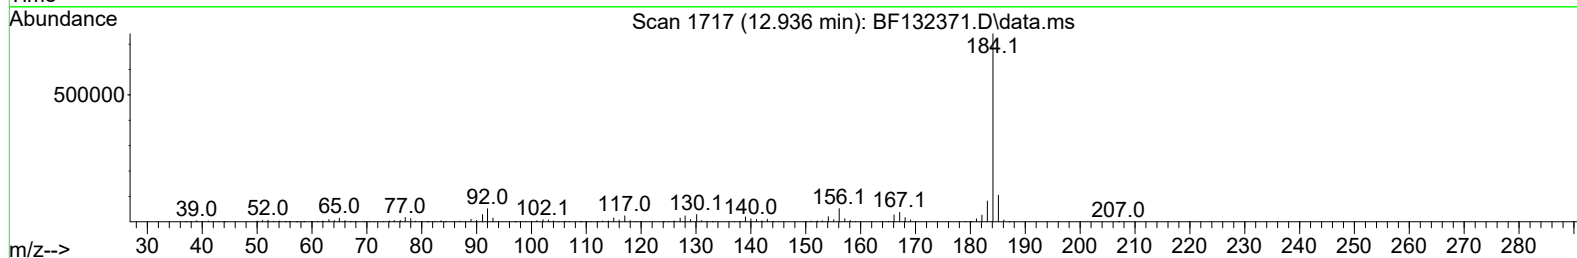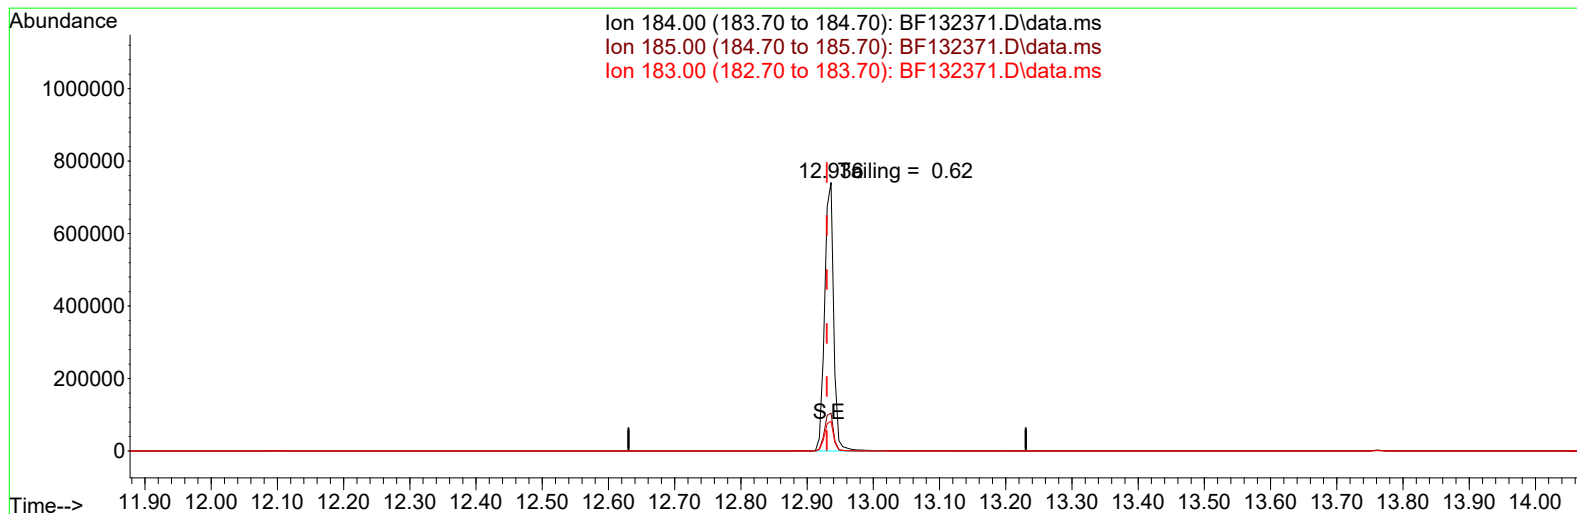

TIC: BF132371.D\data.ms

(77) Benzidine

12.936min (+ 0.006) 0.00 ng

response 705760

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.12
183.00	11.10	11.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2023	BNA_F	<u>BF132371.D</u>
Compound Name	Response	Retention Time
DDT	502001	13.76
DDD	14447	13.46
DDE	1089	13.118
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15536	517537	3.00

Instrument :
BNA_F
ClientSampleId :
DFTPP