
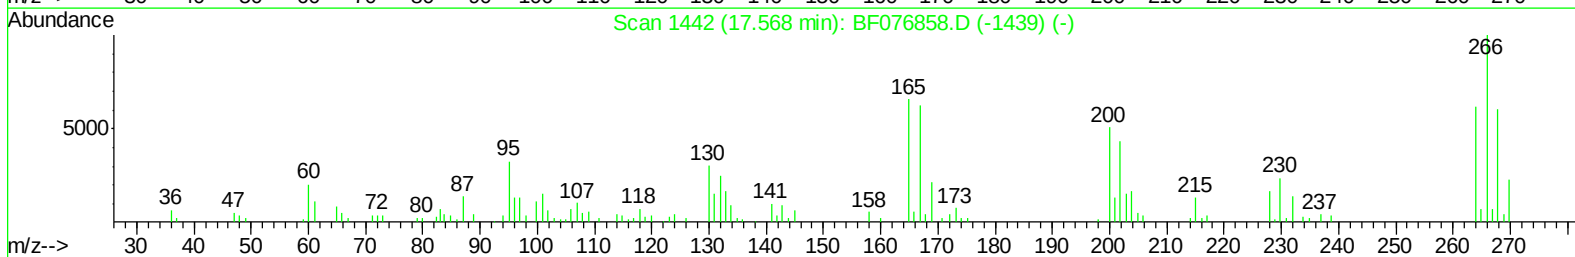
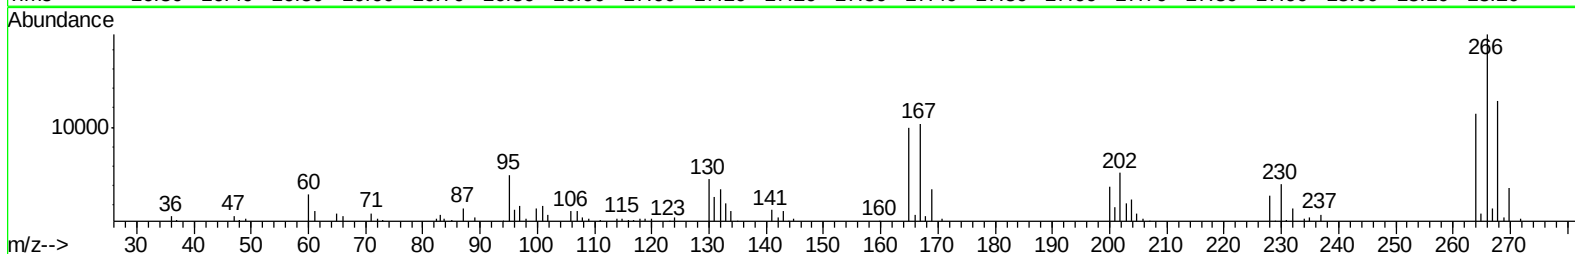


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021015\
Data File : BF077233.D
Acq On : 10 Feb 2015 11:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 00:25:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

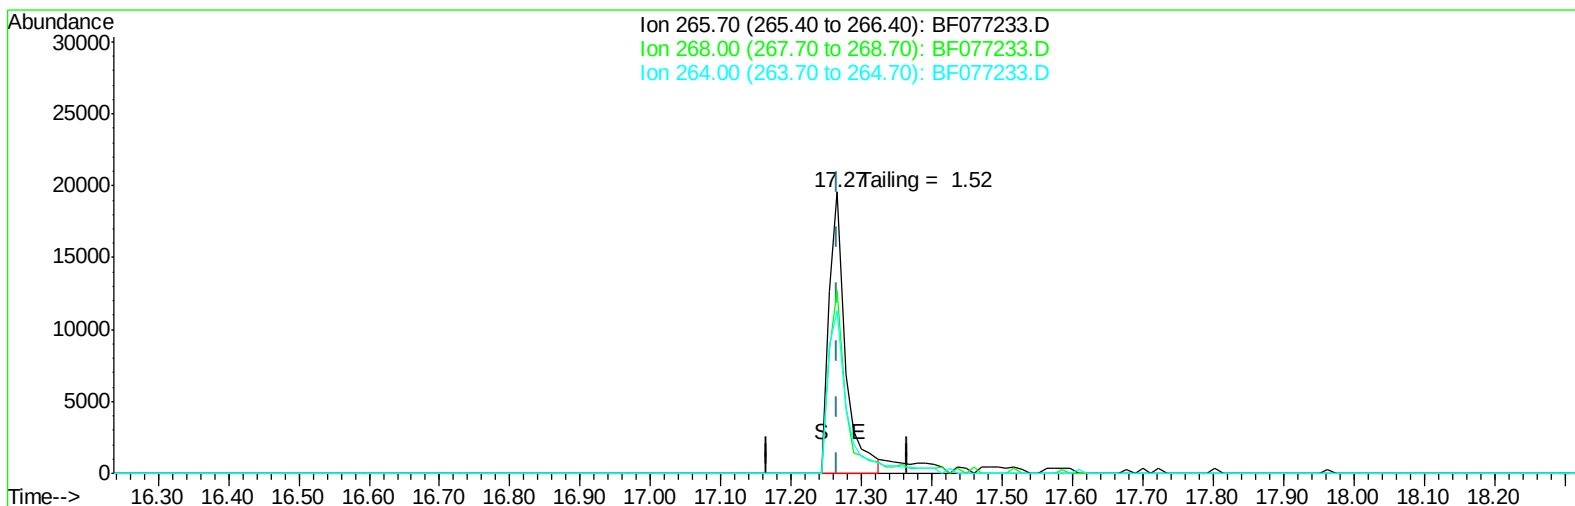

TIC: BF077233.D

(69) Pentachlorophenol (C)




17.266min (+0.000) 0.00ng

response 31660

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	64.84
264.00	61.90	57.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021015\
Data File : BF077233.D
Acq On : 10 Feb 2015 11:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 00:25:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

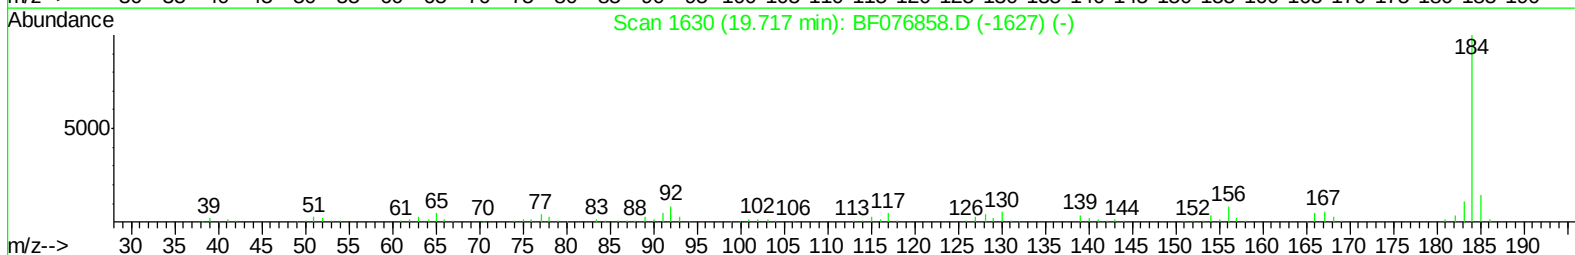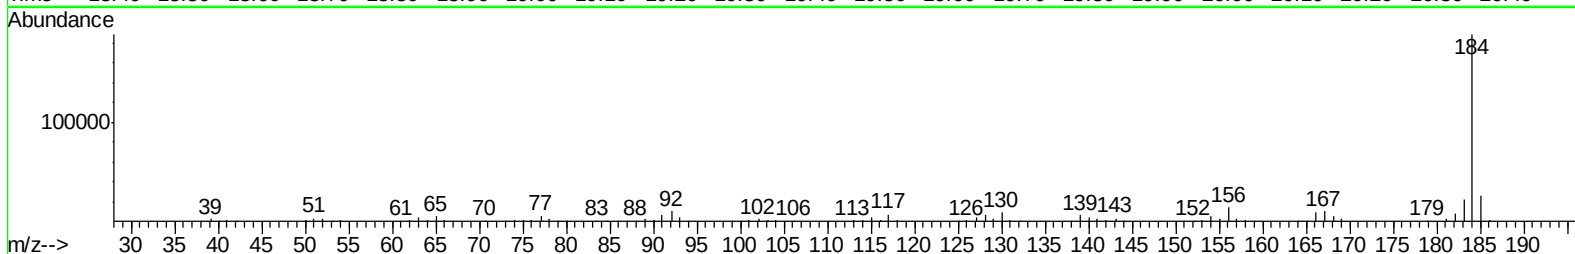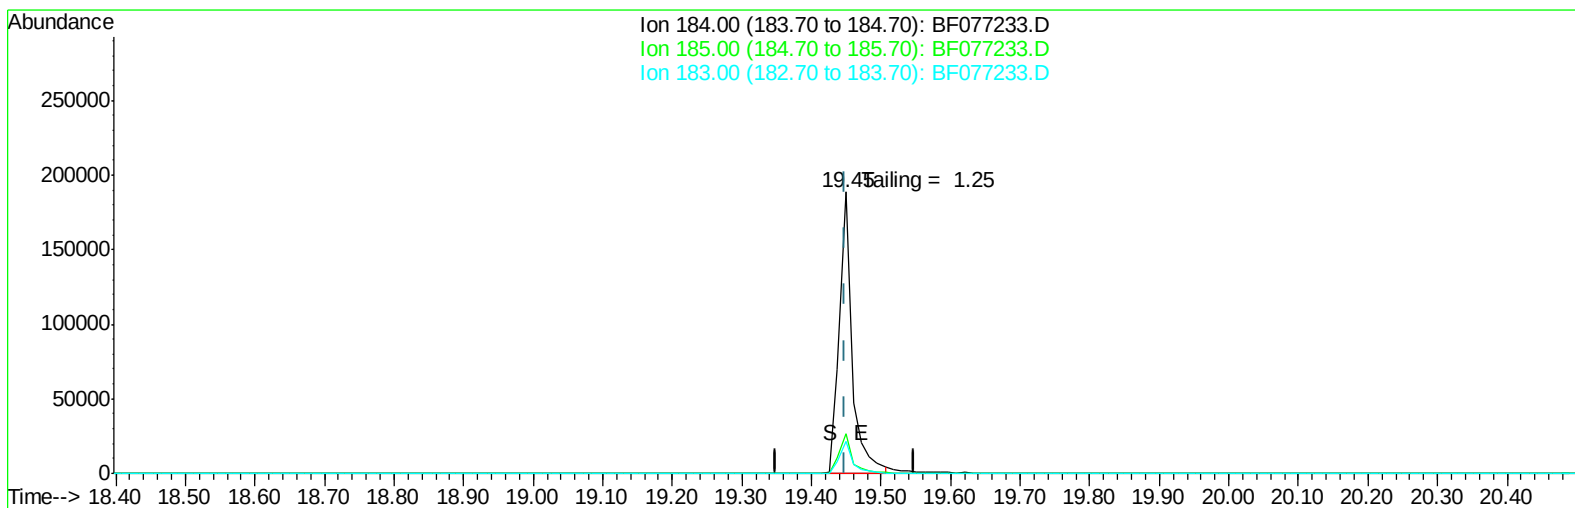

TIC: BF077233.D

(76) Benzidine

19.449min (+0.000) 0.00ng

response 239788

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.91
183.00	11.30	11.60
0.00	0.00	0.00