

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021015\
 Data File : BF077235.D
 Acq On : 10 Feb 2015 13:39
 Operator : TP/IZ
 Sample : G1257-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	39	41	54	rBV	45736	111377	49.95%	8.235%
2	7.596	584	587	594	rBV	65570	118154	52.99%	8.737%
3	10.499	839	841	856	rBB	105027	189931	85.17%	14.044%
4	14.614	1198	1201	1208	rBB	124097	216410	97.05%	16.002%
5	17.506	1451	1454	1459	rBV	161623	221757	99.45%	16.397%
6	21.014	1758	1761	1767	rBB	175652	222992	100.00%	16.489%
7	22.637	1901	1903	1909	rBV	160967	192577	86.36%	14.240%
8	23.083	1938	1942	1944	rBV	1291	3587	1.61%	0.265%
9	23.609	1987	1988	1990	rBV2	1257	2403	1.08%	0.178%
10	23.735	1996	1999	2001	rBV2	2012	4136	1.85%	0.306%
11	24.101	2027	2031	2032	rBV2	1218	2337	1.05%	0.173%
12	24.249	2042	2044	2047	rVV3	1457	2483	1.11%	0.184%
13	24.352	2050	2053	2055	rVB3	2004	4025	1.80%	0.298%
14	24.421	2055	2059	2060	rBV3	2050	4617	2.07%	0.341%
15	24.489	2063	2065	2067	rVB	2060	3269	1.47%	0.242%
16	24.535	2067	2069	2070	rBV	1418	2232	1.00%	0.165%
17	24.661	2078	2080	2082	rBV2	2271	3091	1.39%	0.229%
18	24.741	2085	2087	2089	rBV2	1396	2737	1.23%	0.202%
19	24.775	2089	2090	2093	rBV	1948	2765	1.24%	0.204%
20	24.901	2099	2101	2105	rVB2	1714	3237	1.45%	0.239%
21	24.969	2105	2107	2110	rBV2	1807	4008	1.80%	0.296%
22	25.221	2126	2129	2130	rBV2	1656	2991	1.34%	0.221%
23	25.769	2174	2177	2181	rBV3	1808	5616	2.52%	0.415%
24	25.872	2184	2186	2191	rVB3	1488	3579	1.60%	0.265%
25	26.032	2197	2200	2201	rBV3	1443	3318	1.49%	0.245%
26	26.158	2208	2211	2214	rVB2	2421	6462	2.90%	0.478%
27	26.421	2231	2234	2236	rBV3	1013	2307	1.03%	0.171%
28	26.604	2249	2250	2253	rBV	1262	2252	1.01%	0.167%
29	26.958	2280	2281	2283	rVB	2002	2492	1.12%	0.184%
30	27.118	2291	2295	2297	rBV3	1508	2540	1.14%	0.188%
31	27.152	2297	2298	2301	rVB2	1651	2727	1.22%	0.202%


Sum of corrected areas: 1352409

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021015\
Data File : BF077235.D
Acq On : 10 Feb 2015 13:39
Operator : TP/IZ
Sample : G1257-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

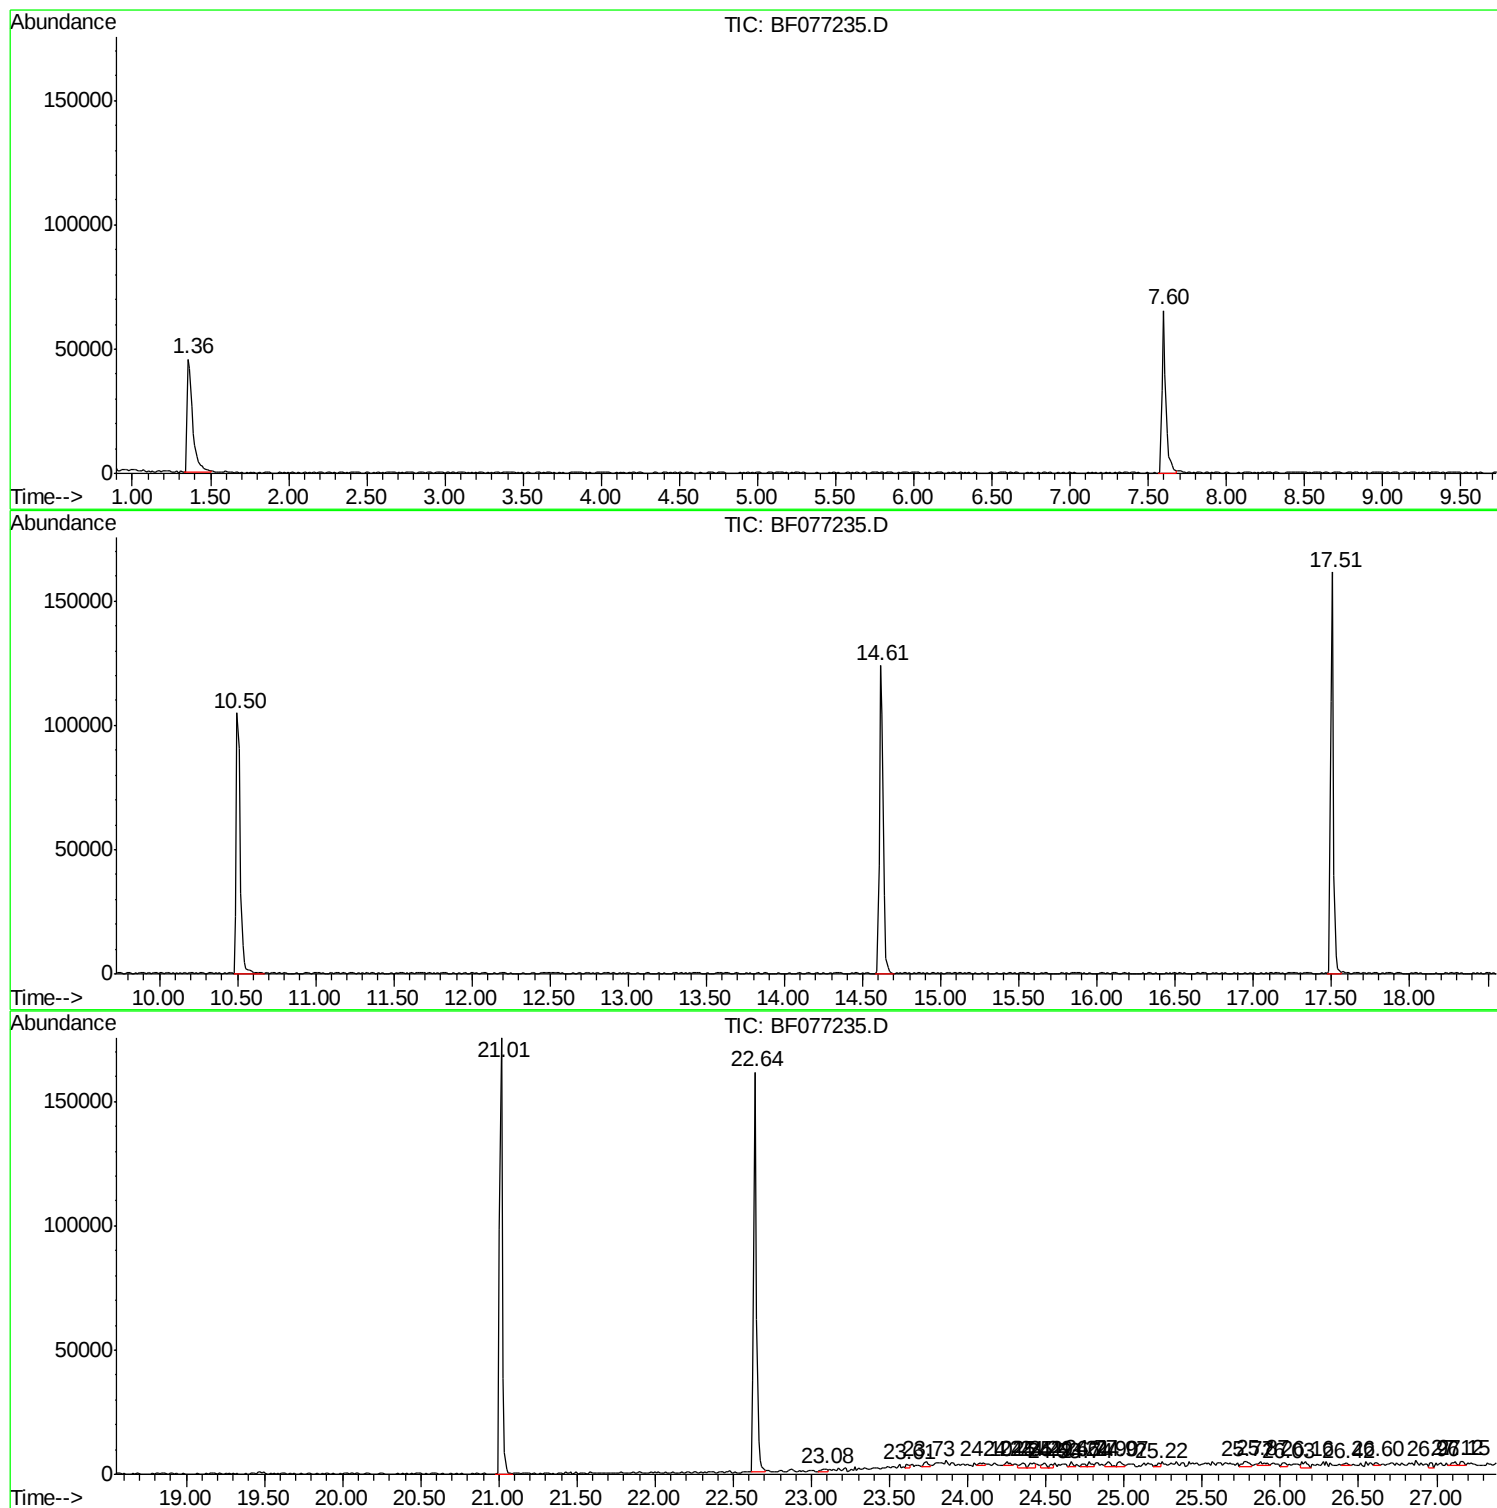

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF021015\
Data_File : BF077235.D
Acq_On : 10_Feb_2015_ 13:399
Operator : TP/IZZ
Sample : G1257-055
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	-Internal Standard-	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---------------------	---	----	------	------

No Library Search Compounds Detected
