


Data Path : Z:\HPCHEM1\BNA F\Data\BF021015\
 Data File : BF077233.D
 Acq On : 10 Feb 2015 11:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 10 13:30:38 2015

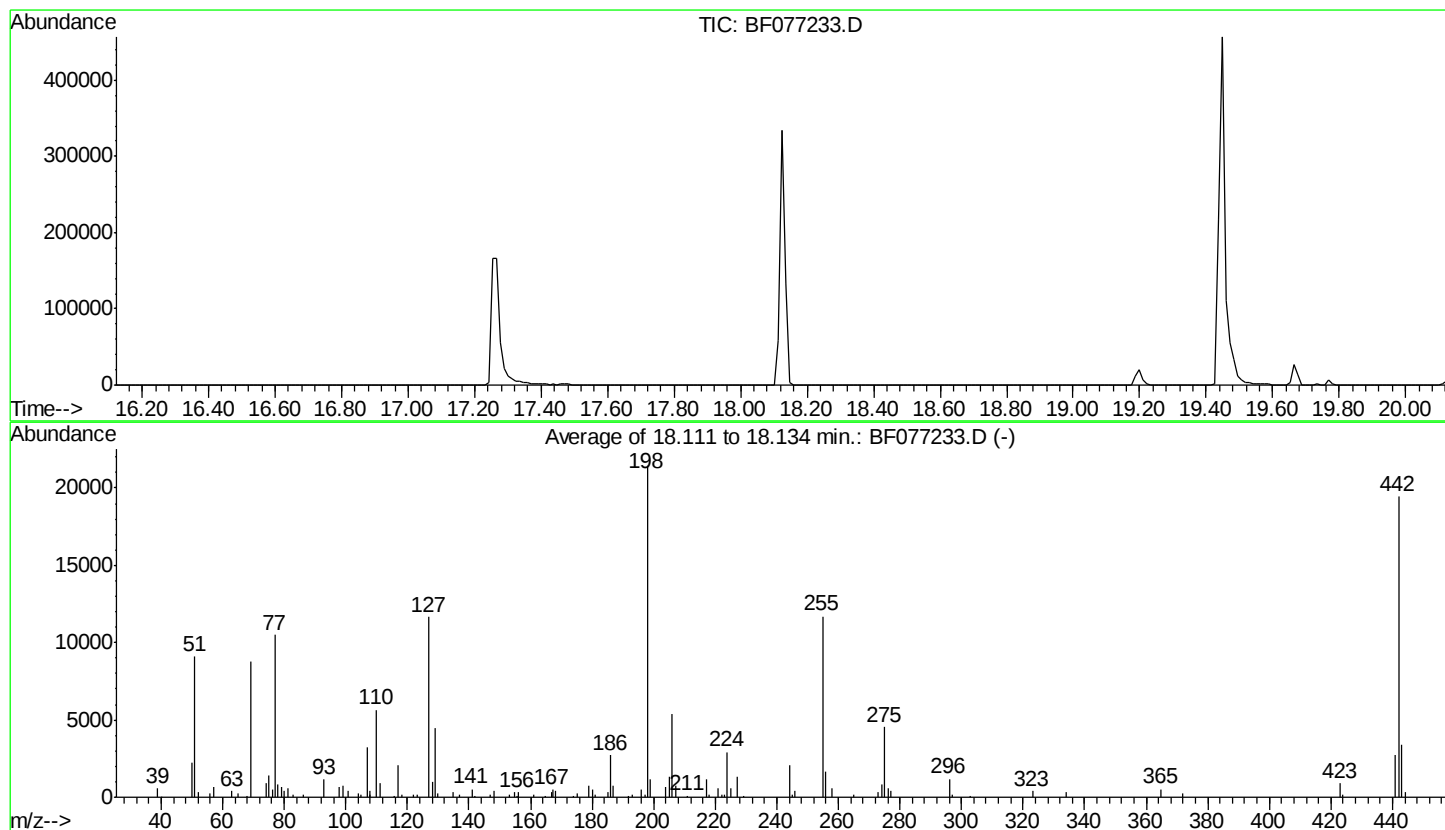

AutoFind: Scans 1507, 1508, 1509; Background Corrected with Scan 1504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	9074	PASS
68	69	0.00	2	1.3	111	PASS
69	198	0.00	100	40.9	8775	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	11661	PASS
197	198	0.00	2	0.7	143	PASS
198	198	100	100	100.0	21445	PASS
199	198	5	9	5.6	1197	PASS
275	198	10	60	21.2	4536	PASS
365	198	1	100	2.3	501	PASS
441	442	0.01	24	14.2	2756	PASS
442	198	50	100	90.6	19424	PASS
443	442	15	24	17.6	3413	PASS