

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
 Data File : BF084994.D
 Acq On : 10 Feb 2016 15:48
 Operator : SJ/IZ
 Sample : H1392-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-5W-(0-2)RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.633	3	4	9	rBV	110812	171478	1.09%	0.426%
2	1.747	9	14	18	rVV2	526029	1144632	7.28%	2.842%
3	1.804	18	19	29	rVB	99343	158642	1.01%	0.394%
4	4.822	275	283	285	rBV	4864426	15717238	100.00%	39.023%
5	5.210	316	317	326	rBV	160747	235345	1.50%	0.584%
6	6.273	408	410	412	rBV	1801668	1588607	10.11%	3.944%
7	6.387	418	420	423	rVB	721586	584209	3.72%	1.450%
8	6.616	438	440	443	rBV	713139	888023	5.65%	2.205%
9	6.776	452	454	457	rBV	3160124	3119575	19.85%	7.745%
10	7.199	488	491	493	rBV	2955810	3282410	20.88%	8.150%
11	7.908	551	553	557	rVB	1231696	1217480	7.75%	3.023%
12	8.993	645	648	650	rBV	3917696	3683214	23.43%	9.145%
13	9.393	680	683	685	rVV	1075142	932614	5.93%	2.316%
14	9.656	703	706	708	rVV	1128750	1266583	8.06%	3.145%
15	10.582	784	787	790	rBV	143262	196664	1.25%	0.488%
16	11.131	833	835	839	rBV	759441	1139841	7.25%	2.830%
17	12.719	972	974	977	rVB	2174752	2296117	14.61%	5.701%
18	12.857	983	986	988	rBV	482538	425736	2.71%	1.057%
19	13.760	1063	1065	1068	rBV	791113	923131	5.87%	2.292%
20	14.080	1090	1093	1095	rVB	405066	363246	2.31%	0.902%
21	15.131	1182	1185	1187	rBV	499824	747054	4.75%	1.855%
22	16.903	1336	1340	1345	rVB7	59042	194652	1.24%	0.483%


Sum of corrected areas: 40276491

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
Data File : BF084994.D
Acq On : 10 Feb 2016 15:48
Operator : SJ/IZ
Sample : H1392-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STOCKPILE-5W-(0-2)RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

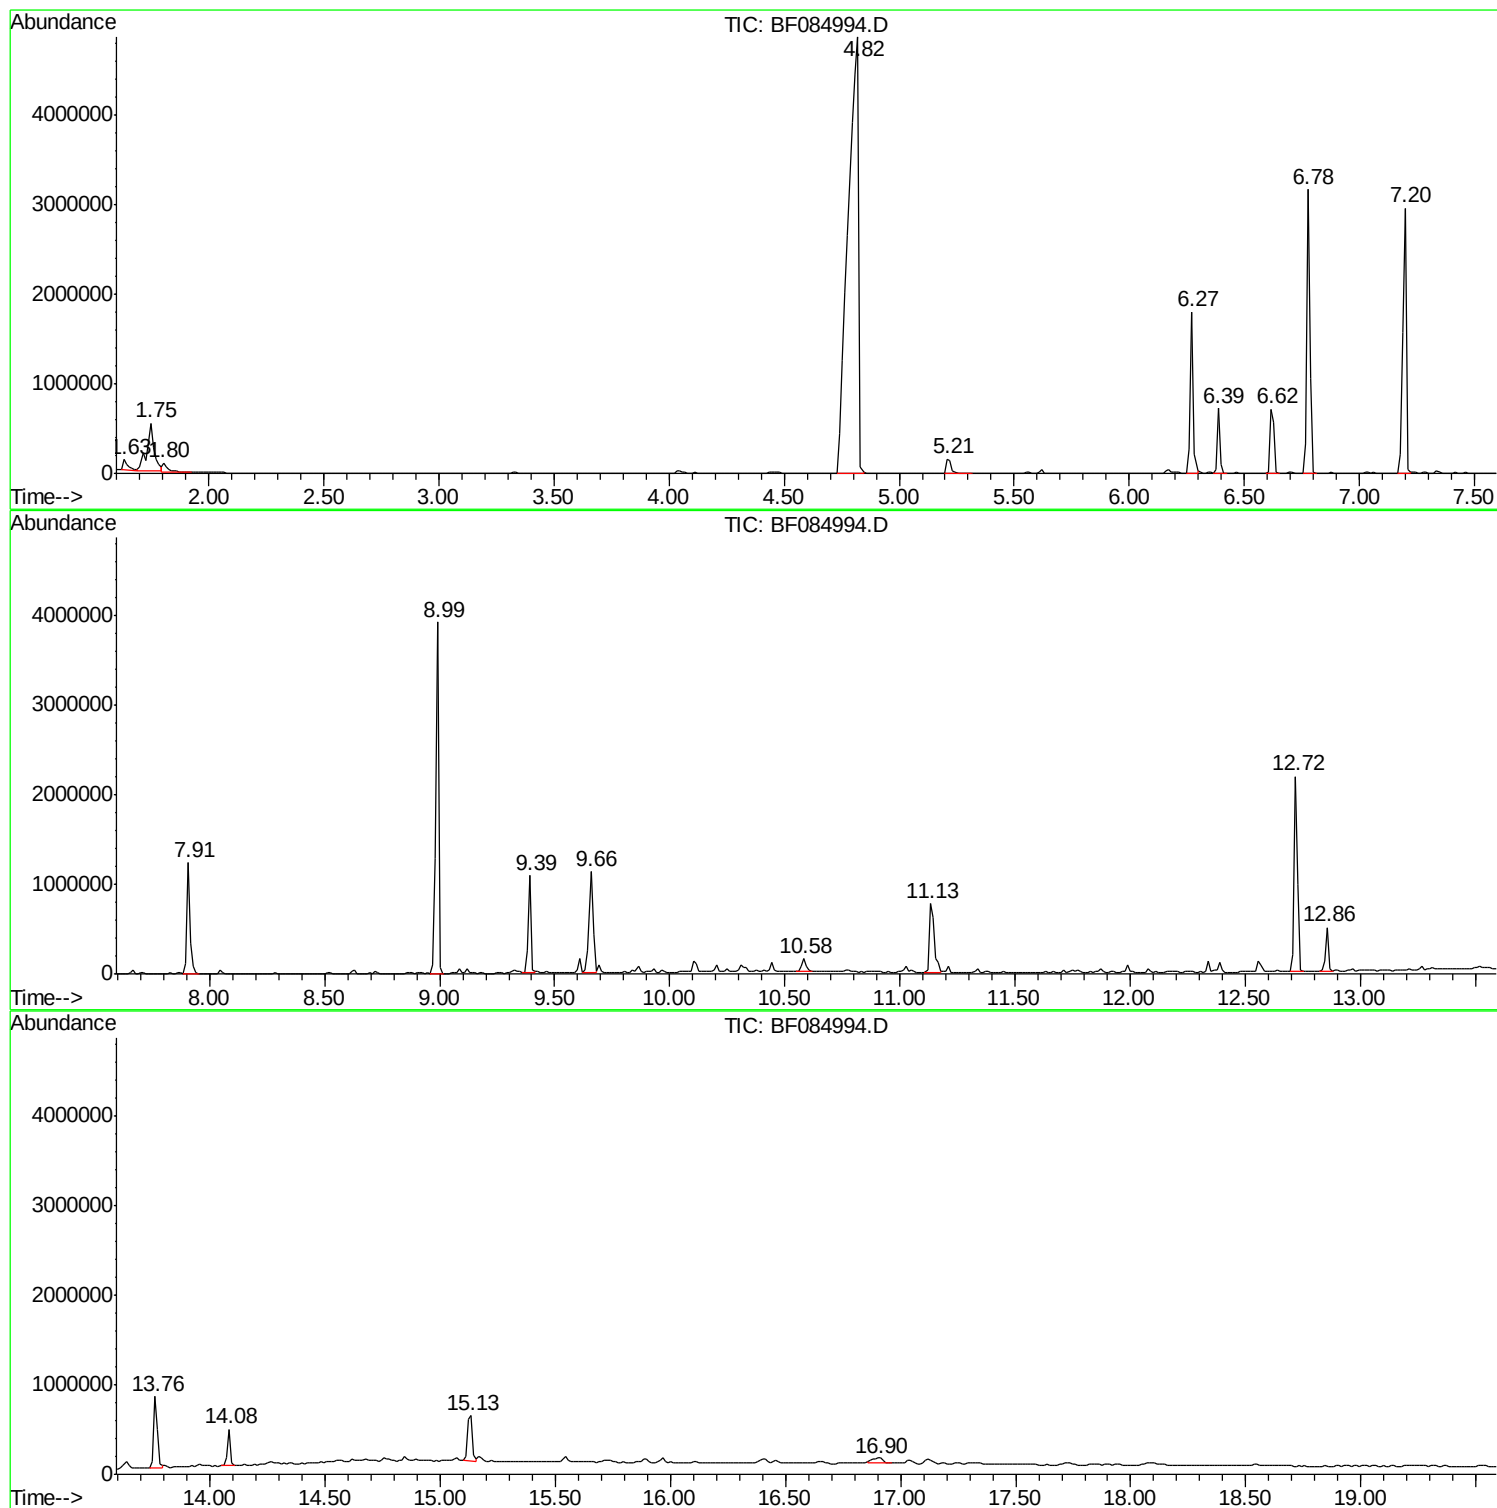

DbaaaPbabbh::ZZ\NRPBHHM1BBAFNDAA\BBO020066\
 DbaaaFfile::BB0000904DD
 Aeqq00n ::100Febb20066 155488
 Oppaaa00r ::SSJIZZ
 Saaapbee ::HH399200RE
 Mmsc ::
 AASSVaal ::88 SaaapbeeMMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-5W-(0-2)RE

QqaabtMebbdd::ZZ\NRPBHHM1BBAFNMEEH00S88200BB0000166MM
 QqaabtTitee ::ASBPBNAASSAANDABBSF00R55P000NTCAILBRATION

TICCLibbaayy ::CC\DAABAASSEN0\$S002LL
 TICInteggaafionPaaameteess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
