

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
 Data File : BF084995.D
 Acq On : 10 Feb 2016 16:16
 Operator : SJ/IZ
 Sample : H1375-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-001(0-2)RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.678	6	8	12	rVB	174391	225130	2.06%	0.116%
2	1.747	12	14	30	rVB	524676	904819	8.28%	0.465%
3	4.661	262	269	272	rBV2	105071	191571	1.75%	0.098%
4	4.753	272	277	284	rBV	850642	1618421	14.81%	0.831%
5	4.947	292	294	296	rBV	175023	253014	2.32%	0.130%
6	5.164	311	313	315	rVB	142225	157991	1.45%	0.081%
7	5.210	315	317	319	rBV	3638315	4276995	39.14%	2.197%
8	5.244	319	320	324	rVB2	149938	208475	1.91%	0.107%
9	5.336	326	328	331	rBV2	319925	381736	3.49%	0.196%
10	5.382	331	332	334	rVB	229182	308436	2.82%	0.158%
11	5.427	334	336	340	rVB3	203177	415862	3.81%	0.214%
12	5.507	340	343	345	rBV	236390	267554	2.45%	0.137%
13	5.610	347	352	354	rBV2	656941	1211089	11.08%	0.622%
14	5.679	354	358	359	rBV2	269782	726368	6.65%	0.373%
15	5.747	362	364	367	rVB2	795715	1159088	10.61%	0.595%
16	5.816	367	370	372	rBV4	528643	1115674	10.21%	0.573%
17	5.862	372	374	377	rVB3	1905731	3034977	27.77%	1.559%
18	5.919	377	379	380	rBV	1651021	1797046	16.44%	0.923%
19	5.942	380	381	387	rVB4	708835	1747481	15.99%	0.897%
20	6.056	387	391	394	rBV3	1098825	2478670	22.68%	1.273%
21	6.136	394	398	404	rVB3	1895464	5031525	46.04%	2.584%
22	6.227	404	406	407	rBV	773301	1237929	11.33%	0.636%
23	6.284	407	411	413	rVB	3893834	4787059	43.80%	2.459%
24	6.319	413	414	416	rVB2	953121	905555	8.29%	0.465%
25	6.399	416	421	426	rBV3	5012954	9886486	90.47%	5.077%
26	6.479	426	428	430	rBV2	1532450	2330292	21.32%	1.197%
27	6.593	430	438	439	rBV4	1359238	4610190	42.19%	2.368%
28	6.627	439	441	442	rBV2	1266312	1170720	10.71%	0.601%
29	6.662	442	444	445	rVB	2931653	2749727	25.16%	1.412%
30	6.696	445	447	449	rBV2	847919	1450021	13.27%	0.745%
31	6.787	451	455	459	rVB4	5045519	10300909	94.26%	5.290%
32	6.902	459	465	469	rBV4	2333880	7777076	71.17%	3.994%
33	6.959	469	470	471	rBV	631831	501908	4.59%	0.258%
34	6.993	471	473	474	rBV2	574253	881117	8.06%	0.453%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
Data File : BF084995.D
Acq On : 10 Feb 2016 16:16
Operator : SJ/IZ
Sample : H1375-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-001(0-2)RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	7.027	474	476	477	rBV	1806949	1579915	14.46%	0.811%
36	7.062	477	479	482	rVB2	1297768	1653250	15.13%	0.849%
37	7.187	485	490	493	rBV4	3113656	9538058	87.28%	4.898%
38	7.290	497	499	502	rVB3	1754524	2909768	26.63%	1.494%
39	7.370	502	506	508	rBV2	1820072	4263465	39.01%	2.190%
40	7.450	508	513	516	rVB4	3557734	7630087	69.82%	3.919%
41	7.507	516	518	520	rBV2	861444	1449039	13.26%	0.744%
42	7.565	520	523	527	rBV5	3373915	8305760	76.00%	4.266%
43	7.679	530	533	534	rVV2	1124512	2290877	20.96%	1.177%
44	7.770	538	541	543	rBV3	1462910	3246853	29.71%	1.667%
45	7.930	550	555	557	rBV3	4014362	10928194	100.00%	5.612%
46	8.033	561	564	569	rVB2	3819928	9986249	91.38%	5.129%
47	8.159	569	575	577	rBV5	2494375	8112581	74.24%	4.166%
48	8.399	592	596	599	rBV	4970447	10902955	99.77%	5.599%
49	8.559	608	610	612	rBV2	1505547	3512733	32.14%	1.804%
50	8.993	645	648	653	rVB2	3888801	9693412	88.70%	4.978%
51	10.388	767	770	772	rBV	2901055	4732478	43.31%	2.430%
52	11.108	831	833	836	rVB	3918726	6965255	63.74%	3.577%
53	12.171	923	926	928	rVB2	1503662	3171896	29.02%	1.629%
54	12.228	929	931	933	rVB	1109181	1166887	10.68%	0.599%
55	12.742	974	976	981	rVB	2442647	3559701	32.57%	1.828%
56	13.634	1052	1054	1064	rVB	722866	1300563	11.90%	0.668%
57	13.771	1064	1066	1070	rVB	939557	1002557	9.17%	0.515%
58	15.131	1182	1185	1187	rBV	626829	710463	6.50%	0.365%


Sum of corrected areas: 194713907

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
Data File : BF084995.D
Acq On : 10 Feb 2016 16:16
Operator : SJ/IZ
Sample : H1375-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-001(0-2)RE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

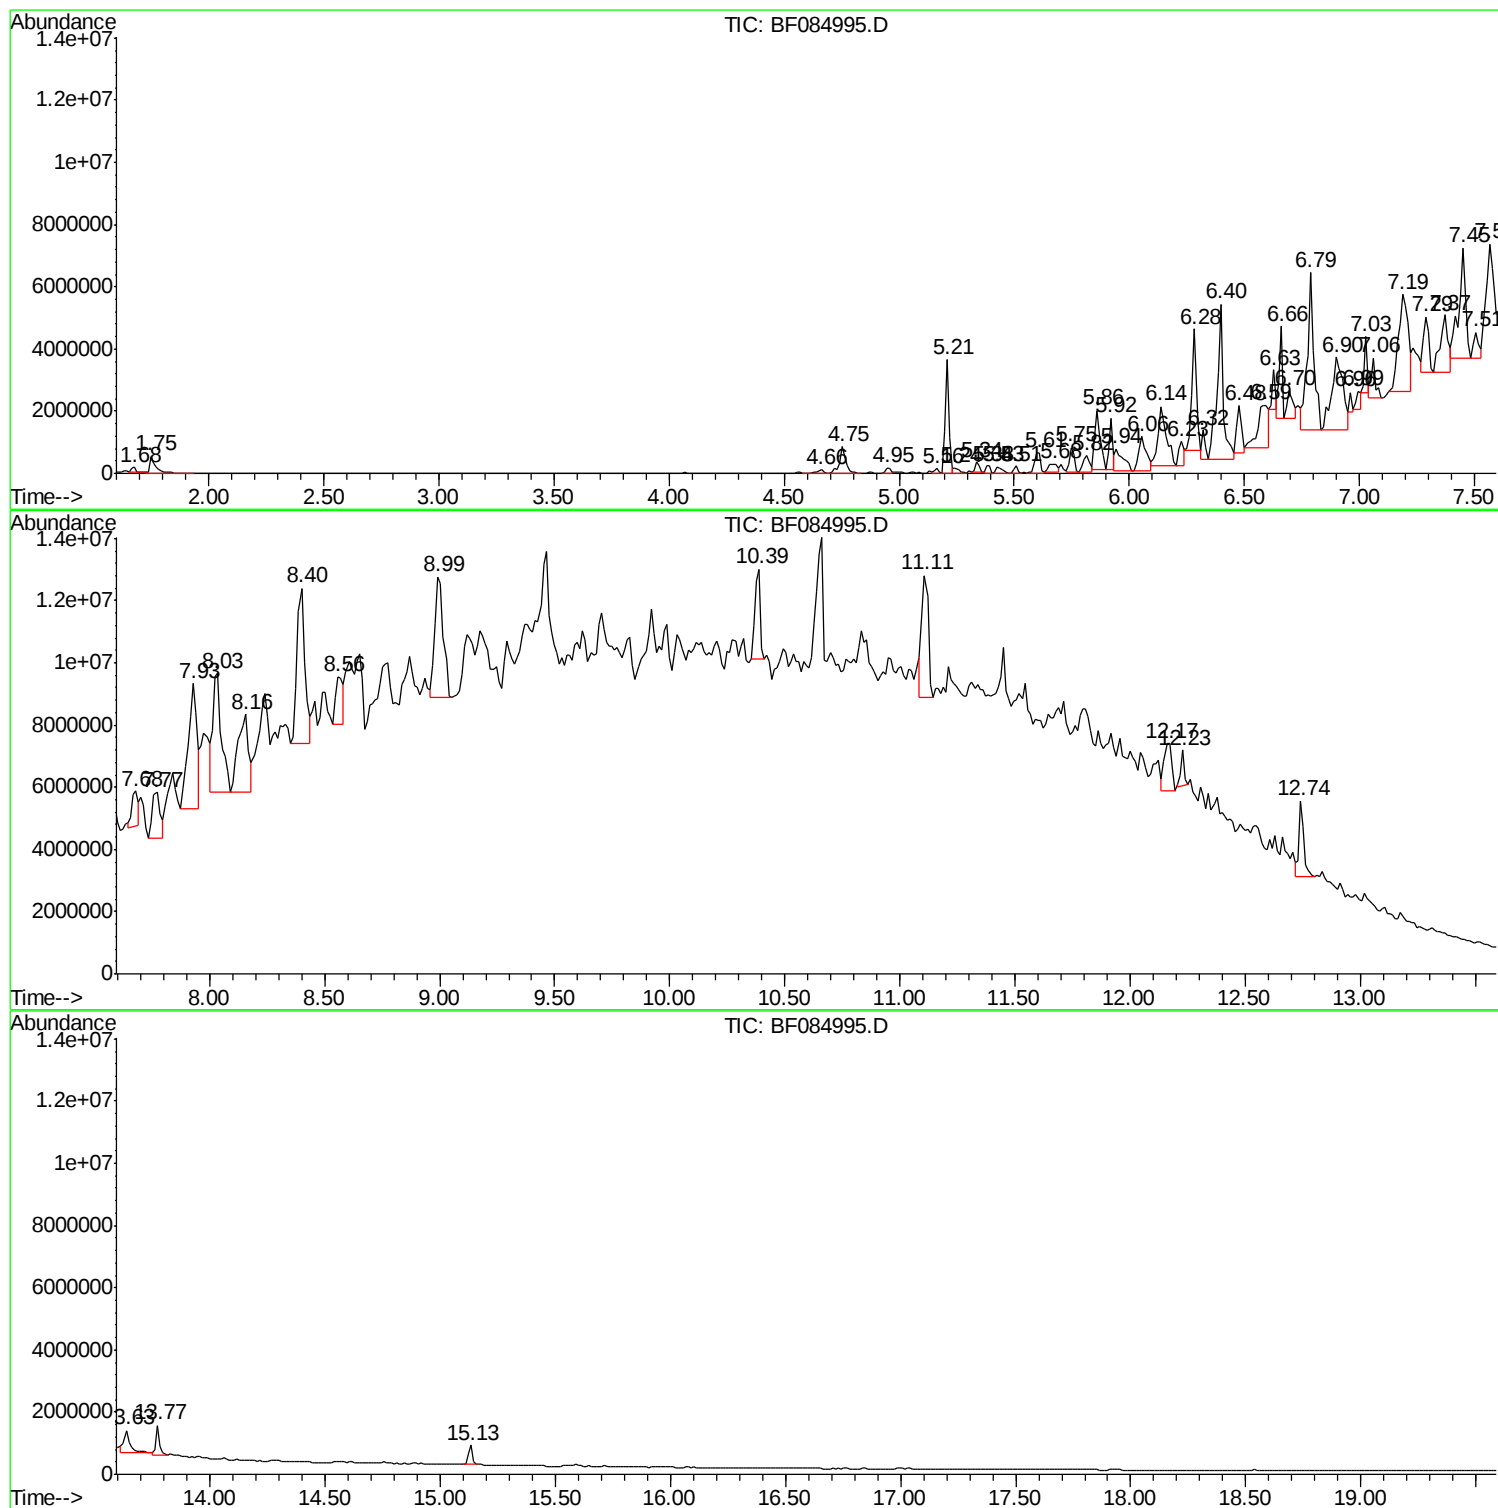

DbaaaPathh::ZZ\NRPBEMM1BBAFNDATA\BBO20066\
 DbaaaFile::BB0030995DD
 Aeqq00n ::100Febb20066 166166
 Oppaaaor ::SSJIZZ
 Saaapbe ::H#3350QRE
 MISC ::
 AASSVaal ::133 SaaapbeMMuipbler:11

Instrument :
 BNA_F
 ClientSampleId :
 SP-001(0-2)RE

QqaabtMebbdd::ZZ\NRPBEMM1BBAFMEH#00S82Z00BB000166MM
 QqaabtTife ::ASBPBNASSANDBBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DATA\BBS6END\$S002LL
 TICInteggaafionPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
