


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021016\
Data File : BF084983.D
Acq On : 10 Feb 2016 10:30
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 10 13:28:51 2016

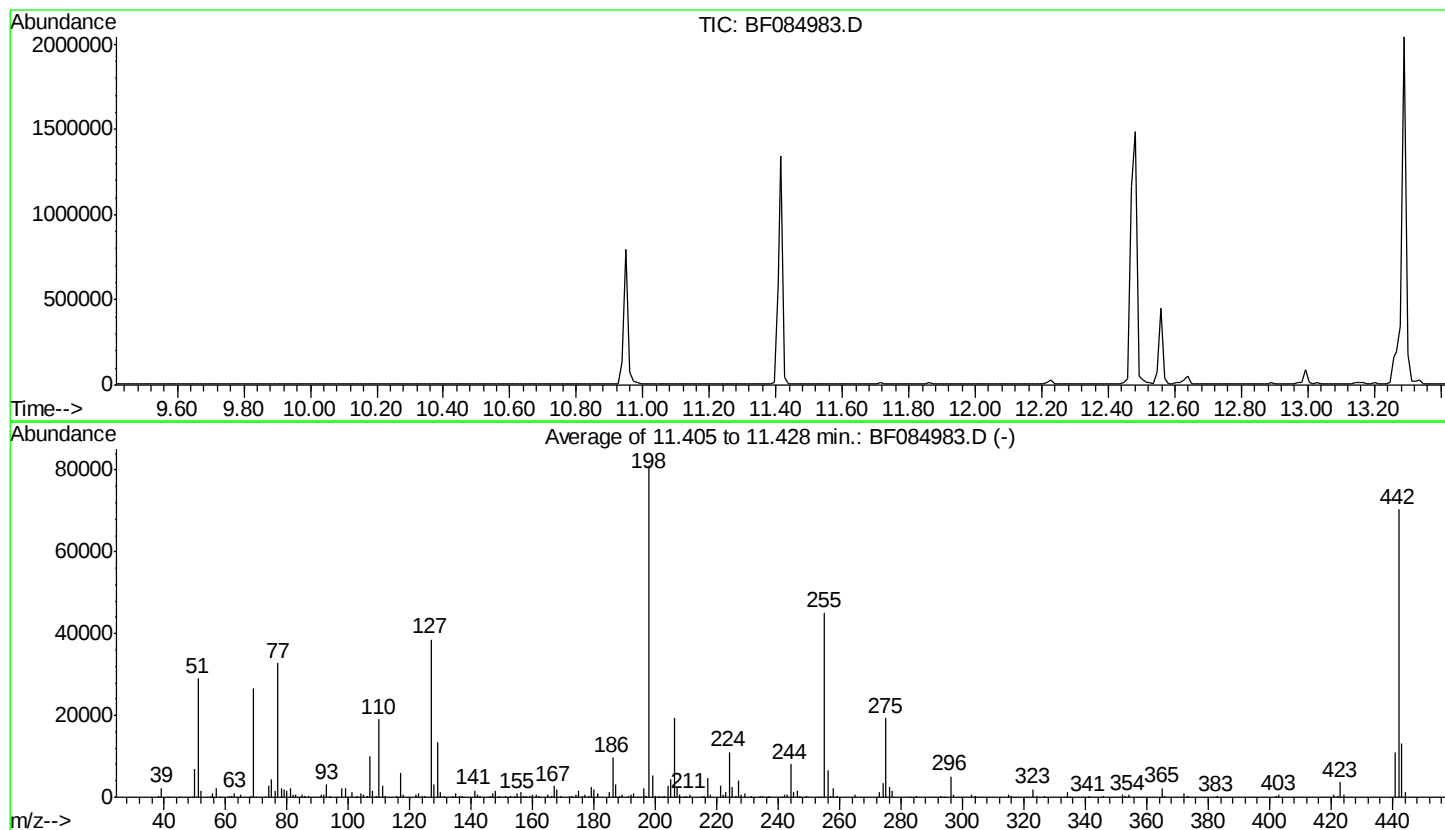

AutoFind: Scans 859, 860, 861; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	29031	PASS
68	69	0.00	2	1.6	418	PASS
69	198	0.00	100	32.7	26496	PASS
70	69	0.00	2	0.4	108	PASS
127	198	10	80	47.6	38575	PASS
197	198	0.00	2	0.5	392	PASS
198	198	100	100	100.0	81073	PASS
199	198	5	9	6.6	5366	PASS
275	198	10	60	23.9	19349	PASS
365	198	1	100	2.8	2298	PASS
441	442	0.01	24	15.7	11029	PASS
442	198	50	100	86.8	70346	PASS
443	442	15	24	18.7	13132	PASS