
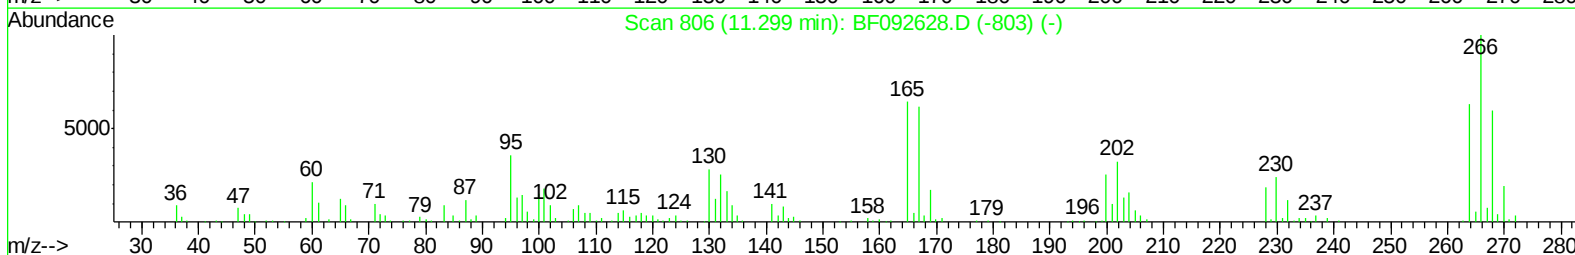
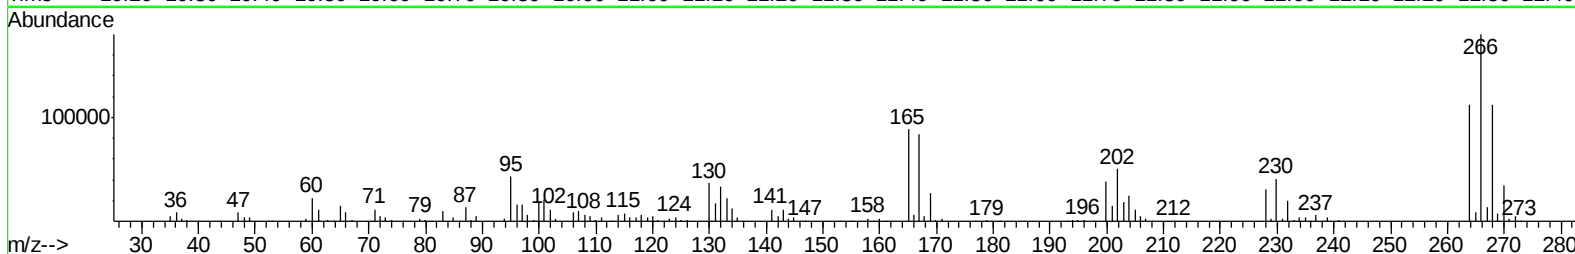


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021017\
Data File : BF092882.D
Acq On : 10 Feb 2017 14:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:46:46 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 23:31:14 2017
Response via : Initial Calibration

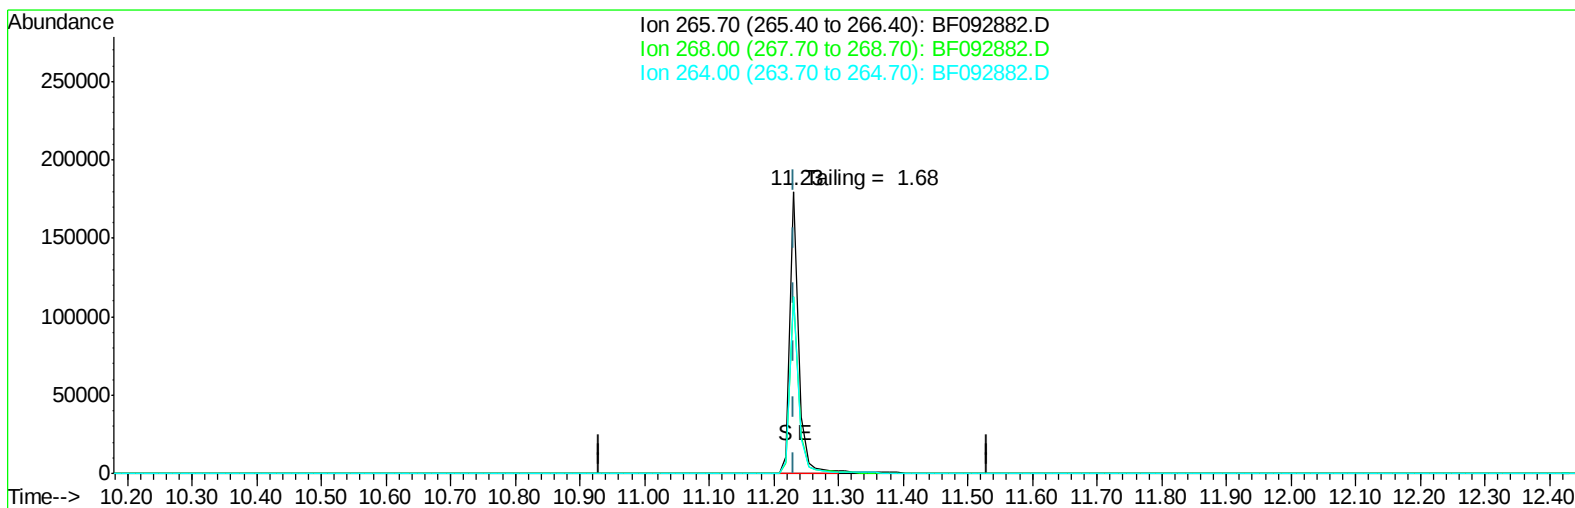

TIC: BF092882.D

(69) Pentachlorophenol (C)




11.231min (+0.000) 0.00ng

response 171226

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.73
264.00	62.90	62.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021017\
Data File : BF092882.D
Acq On : 10 Feb 2017 14:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 03:46:46 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 23:31:14 2017
Response via : Initial Calibration

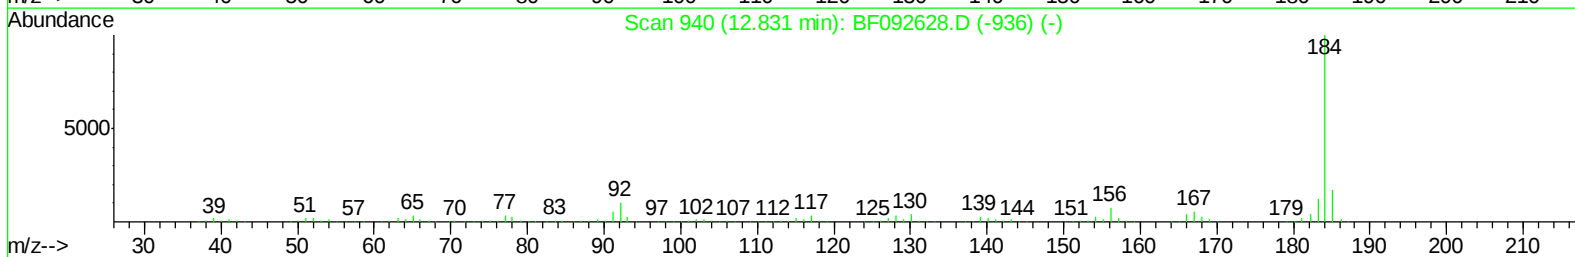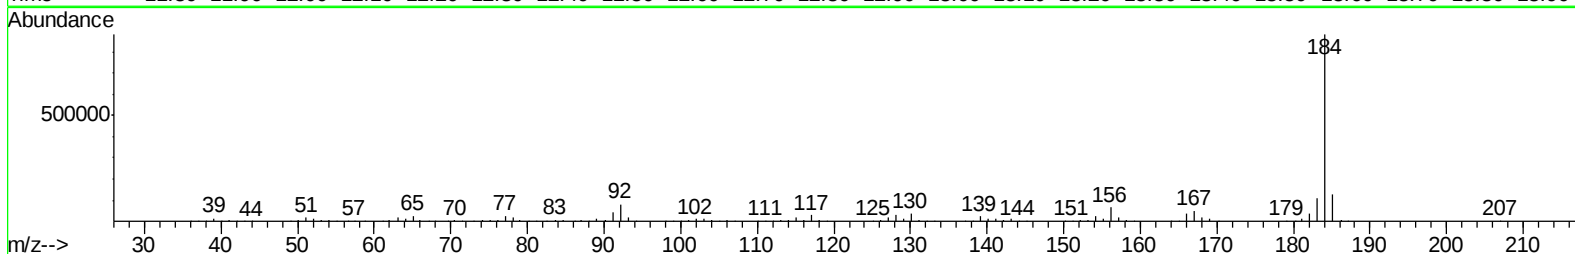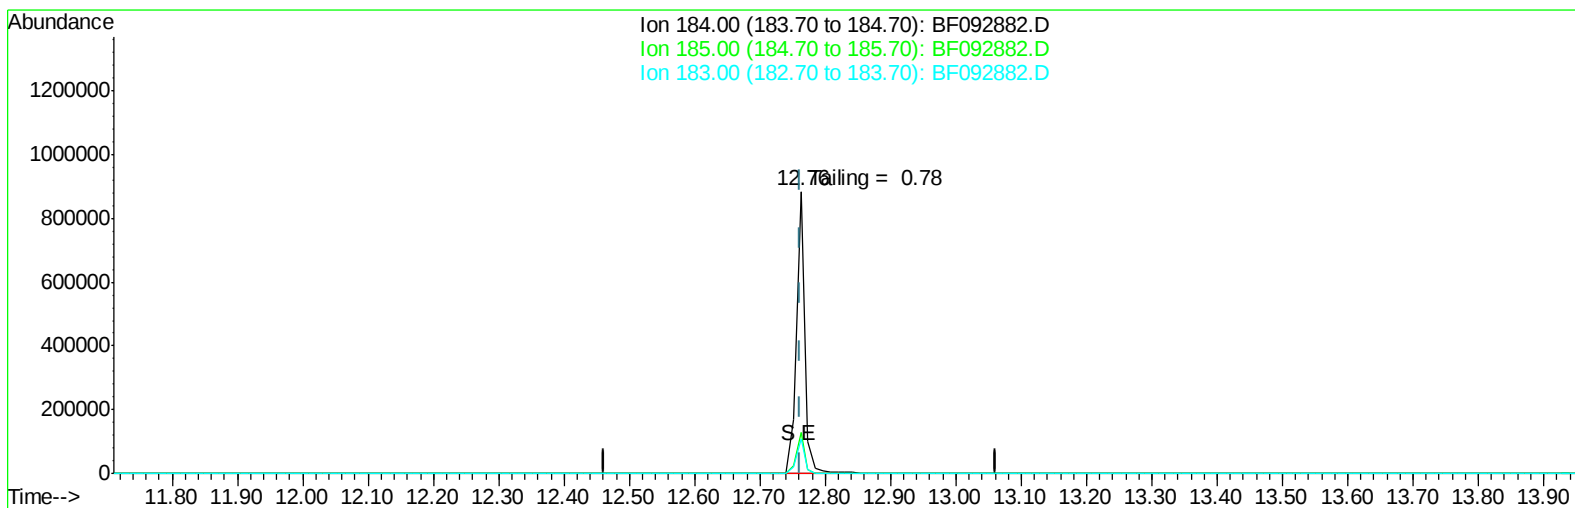

TIC: BF092882.D

(76) Benzidine

12.762min (+0.000) 34332.31ng

response 828054

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.57
183.00	11.50	12.33
0.00	0.00	0.00