

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021017\
 Data File : BF092884.D
 Acq On : 10 Feb 2017 15:51
 Operator : SJ/MA
 Sample : PB96853BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB96853BL

Quant Time: Feb 10 23:36:19 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 10 23:31:14 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	183199	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	745093	20.00	ng	-0.01
38) Acenaphthene-d10	9.94	164	430003	20.00	ng	0.00
63) Phenanthrene-d10	11.42	188	733104	20.00	ng	0.00
75) Chrysene-d12	14.05	240	604247	20.00	ng	-0.01
86) Perylene-d12	15.51	264	510407	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1219510	114.20	ng	0.01
7) Phenol-d6	6.53	99	1446205	105.26	ng	0.00
23) Nitrobenzene-d5	7.46	82	920724	68.81	ng	-0.01
41) 2,4,6-Tribromophenol	10.73	330	330002	106.11	ng	-0.01
44) 2-Fluorobiphenyl	9.26	172	1829281	77.07	ng	0.00
78) Terphenyl-d14	13.01	244	1637345	63.67	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021017\
Data File : BF092884.D
Acq On : 10 Feb 2017 15:51
Operator : SJ/MA
Sample : PB96853BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96853BL

Quant Time: Feb 10 23:36:19 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 10 23:31:14 2017
Response via : Initial Calibration

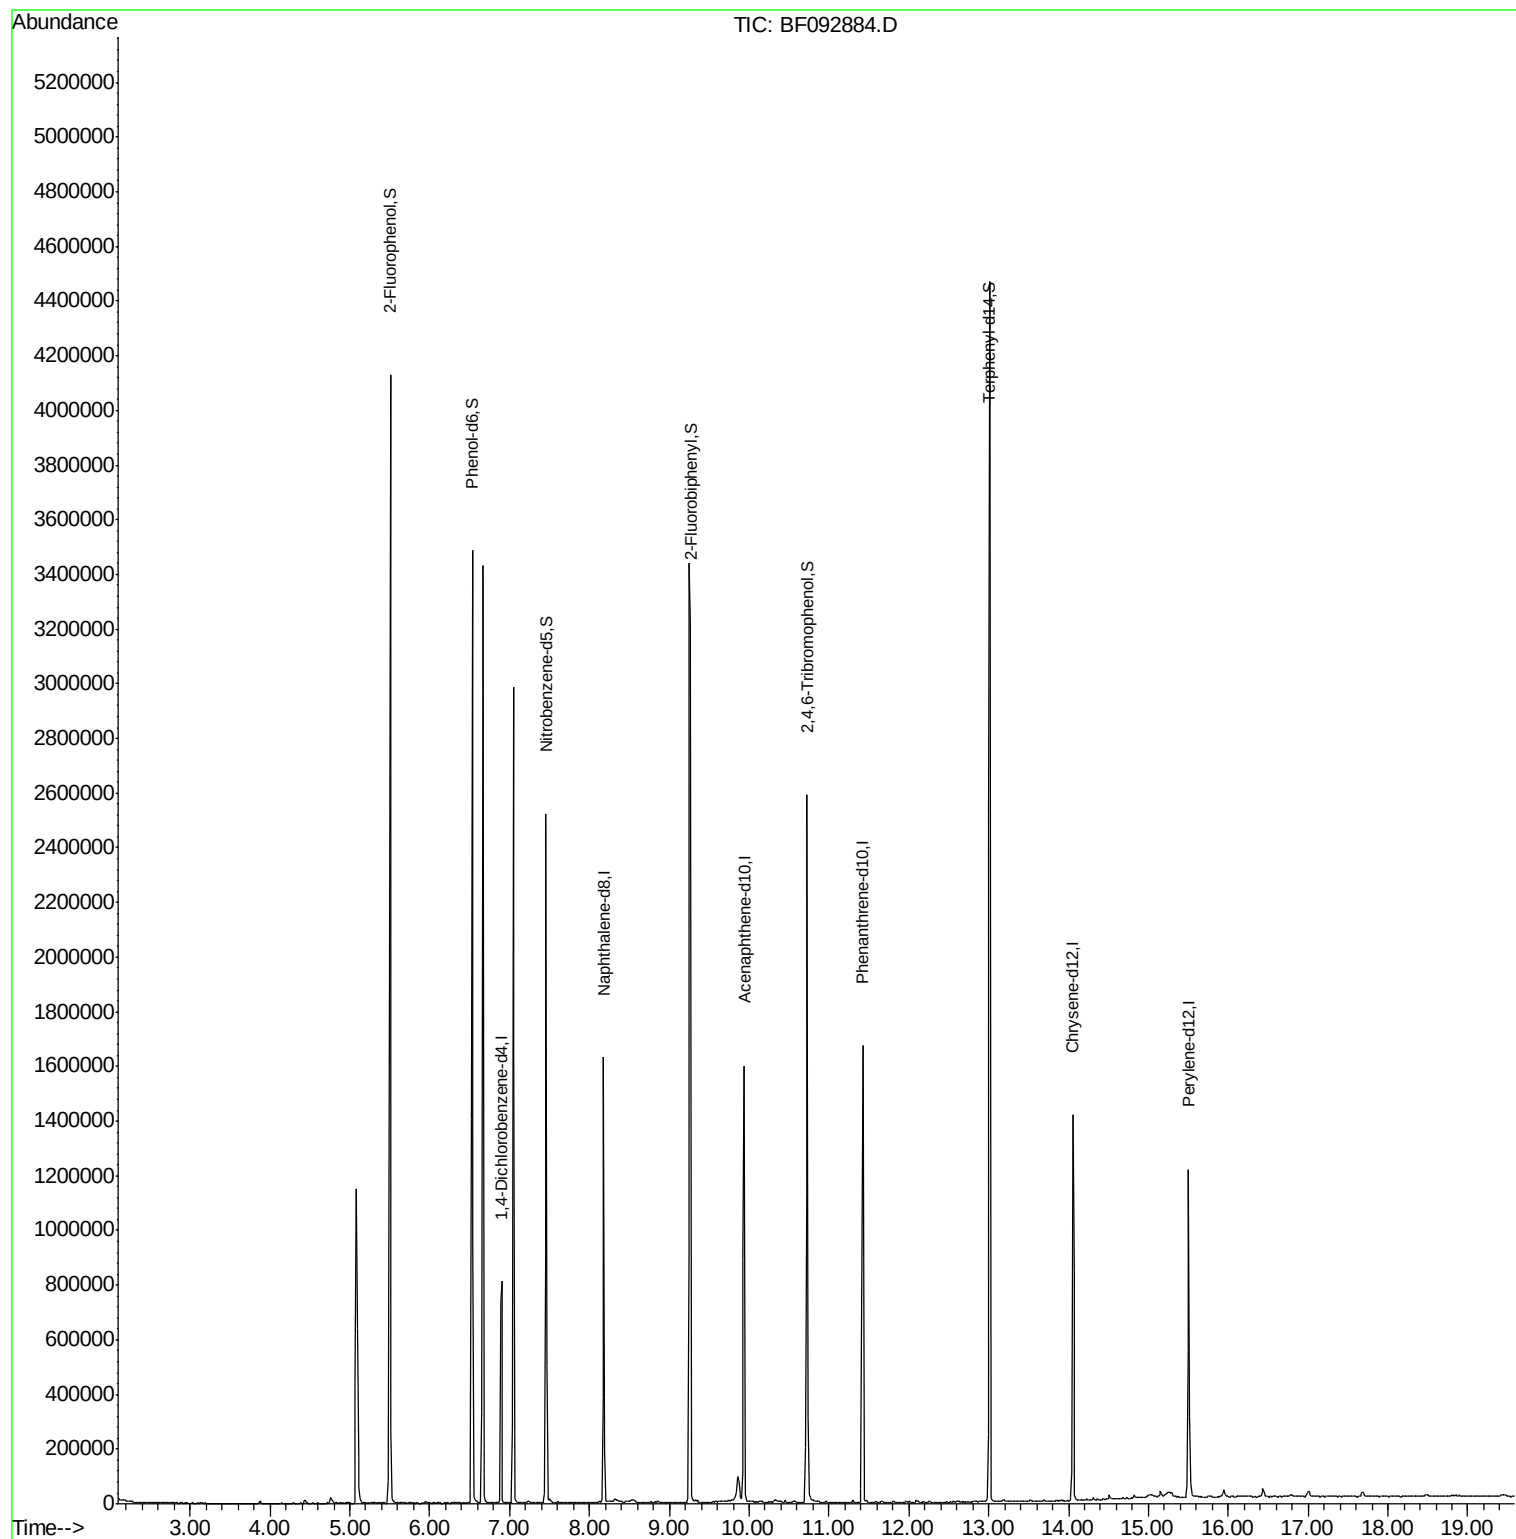

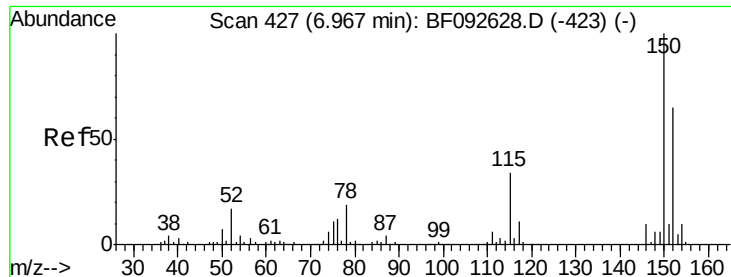

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.90 min Scan# 421

Delta R.T. 0.00 min

Lab File: BF092884.D

Acq: 10 Feb 2017 15:51

Instrument :

BNA_F

ClientSampleId :

PB96853BL


Tgt Ion:152 Resp: 183199

Ion Ratio Lower Upper

152 100

150 151.6 124.9 187.3




115 49.4 46.0 69.0

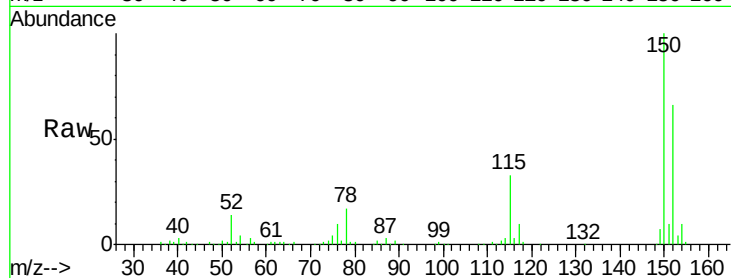

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

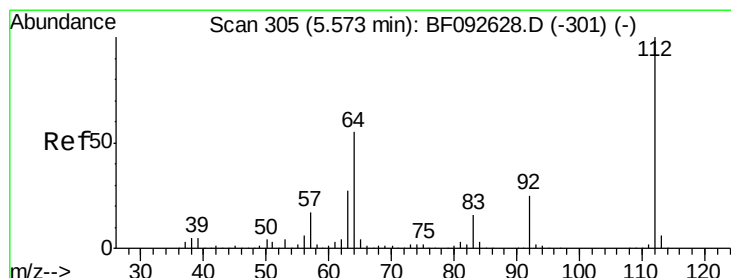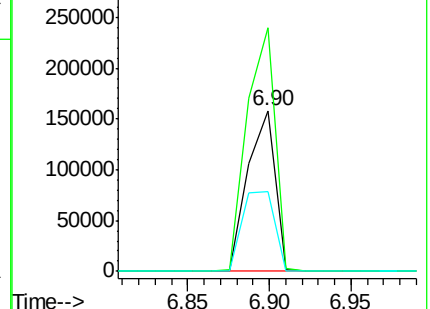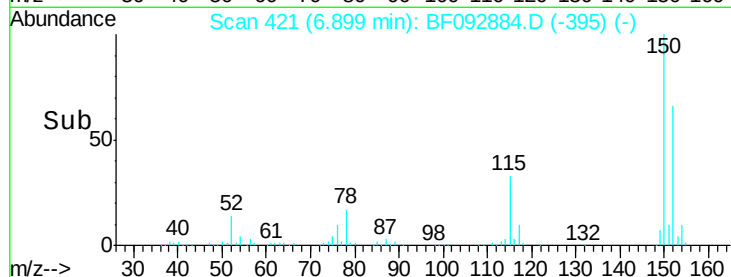

#5

2-Fluorophenol

Concen: 114.20 ng

RT: 5.50 min Scan# 299

Delta R.T. 0.01 min

Lab File: BF092884.D

Acq: 10 Feb 2017 15:51


Tgt Ion:112 Resp: 1219510

Ion Ratio Lower Upper

112 100

64 64.4 46.1 69.1



63 32.6 23.8 35.6

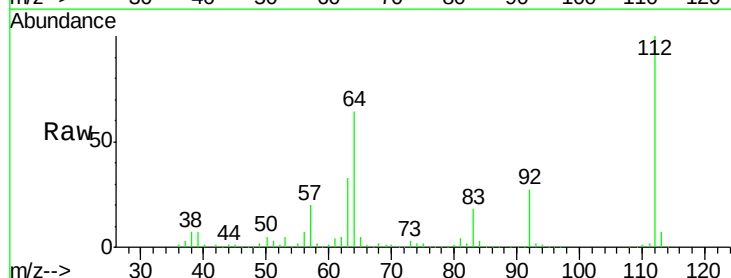


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

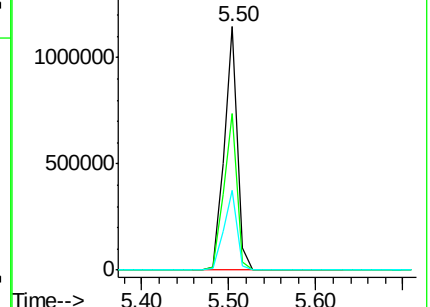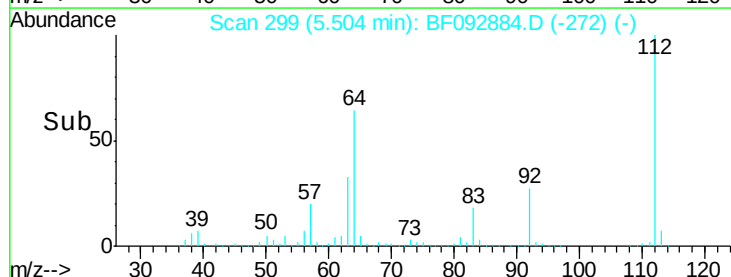

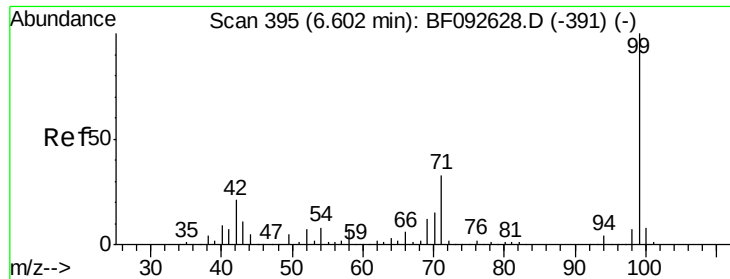

#7

Phenol-d6

Concen: 105.26 ng

RT: 6.53 min Scan# 389

Delta R.T. 0.00 min

Lab File: BF092884.D

Acq: 10 Feb 2017 15:51

Instrument :

BNA_F

ClientSampleId :

PB96853BL


Tgt Ion: 99 Resp: 1446205

Ion Ratio Lower Upper

99 100

42 20.9 15.6 23.4




71 33.7 27.5 41.3

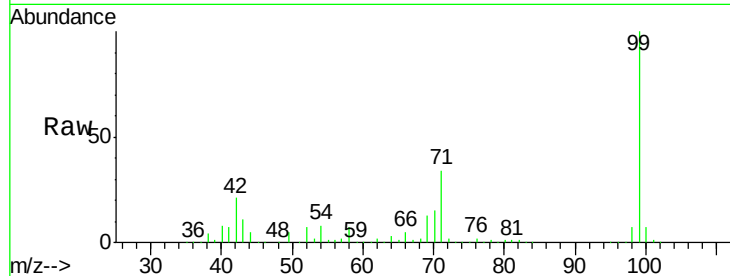

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

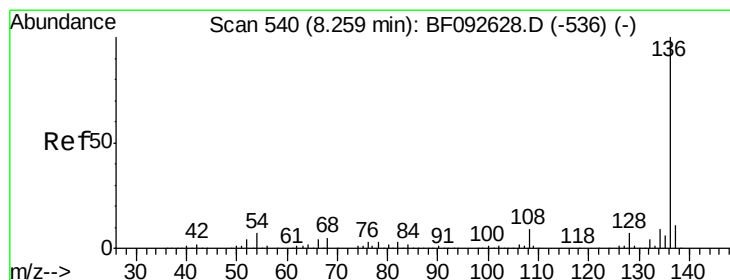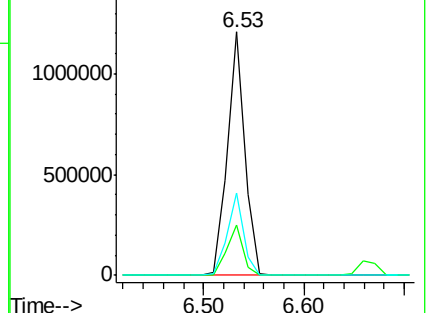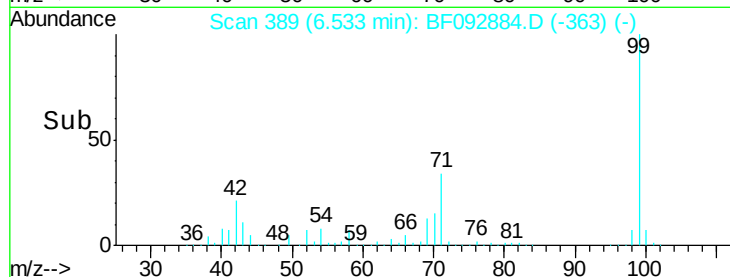

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.18 min Scan# 533

Delta R.T. -0.01 min

Lab File: BF092884.D

Acq: 10 Feb 2017 15:51

Tgt Ion: 136 Resp: 745093


Ion Ratio Lower Upper

136 100

137 11.1 8.4 12.6

54 10.5 4.5 6.7#

68 7.0 3.6 5.4#


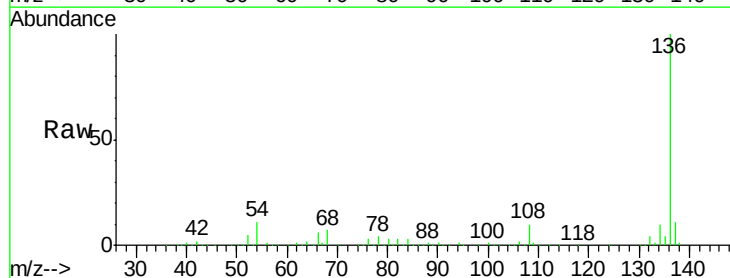



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

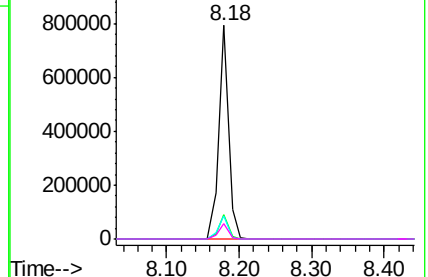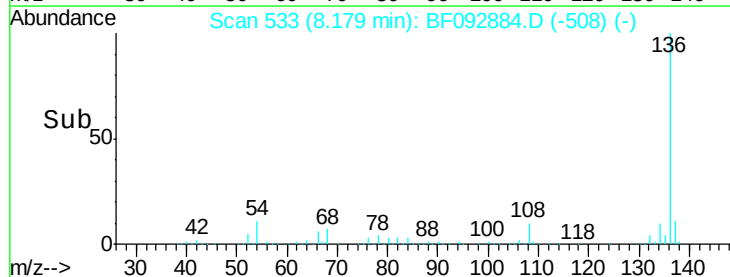


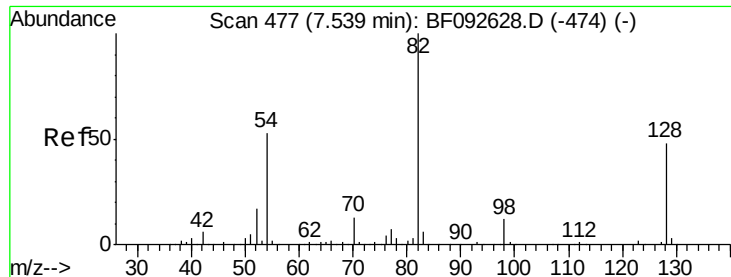




#23
 Nitrobenzene-d5
 Concen: 68.81 ng
 RT: 7.46 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Instrument :
 BNA_F
 ClientSampleId :
 PB96853BL

Tgt Ion: 82 Resp: 920724
 Ion Ratio Lower Upper
 82 100
 128 41.9 34.6 52.0
 54 57.6 39.5 59.3

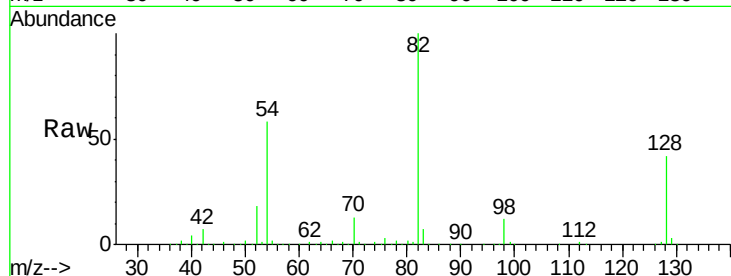


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

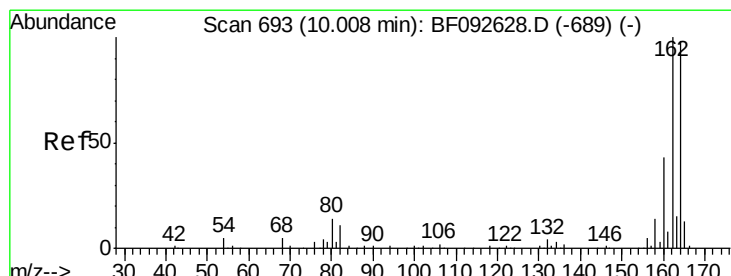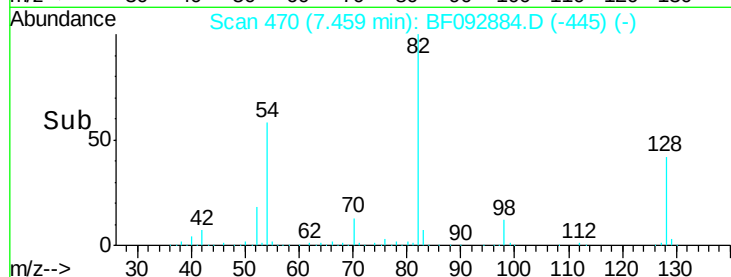
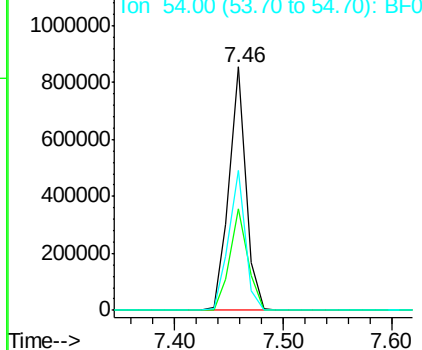



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.94 min Scan# 687
 Delta R.T. 0.00 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Tgt Ion: 164 Resp: 430003
 Ion Ratio Lower Upper
 164 100
 162 101.8 80.2 120.2
 160 42.9 36.9 55.3

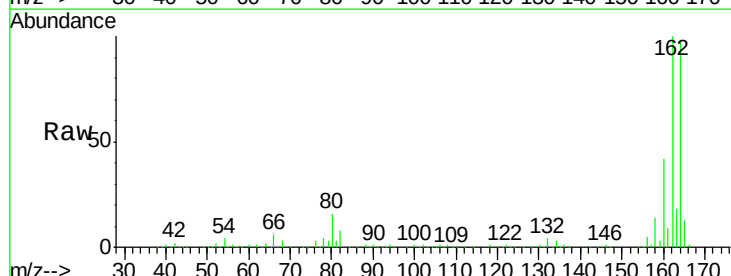

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

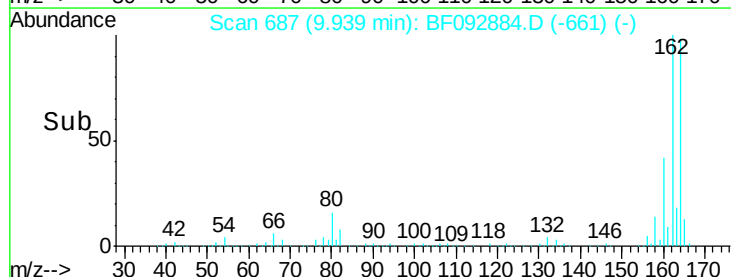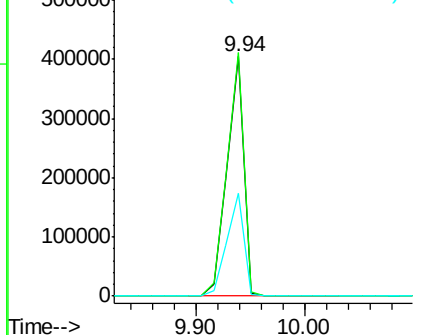


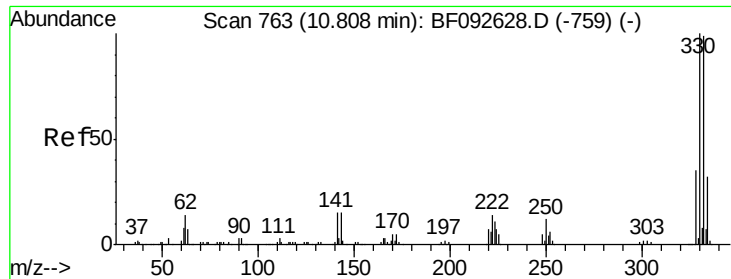




#41
 2,4,6-Tribromophenol
 Concen: 106.11 ng
 RT: 10.73 min Scan# 756
 Delta R.T. -0.01 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Instrument :
 BNA_F
 ClientSampleId :
 PB96853BL

Tgt Ion	Ratio	Lower	Upper
330	100		
332	99.6	77.4	116.2
141	40.9	34.1	51.1

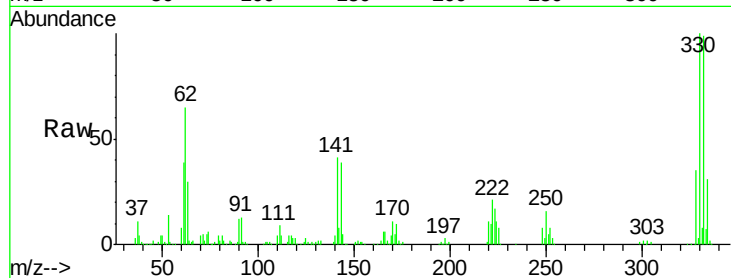


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

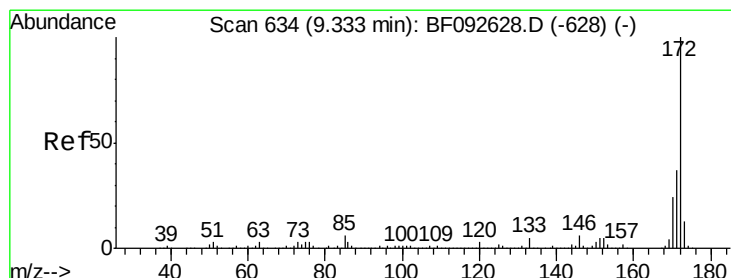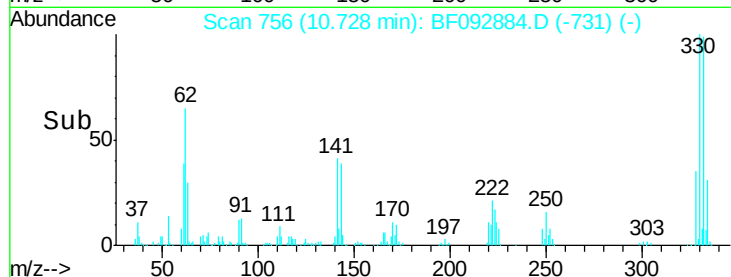
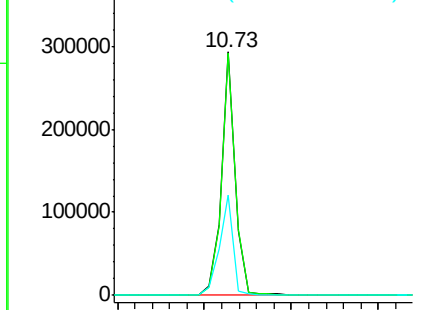



#44
 2-Fluorobiphenyl
 Concen: 77.07 ng
 RT: 9.26 min Scan# 628
 Delta R.T. 0.00 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.4	44.0
170	23.8	20.2	30.4

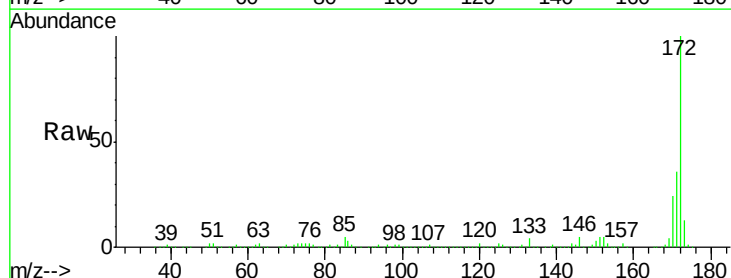

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

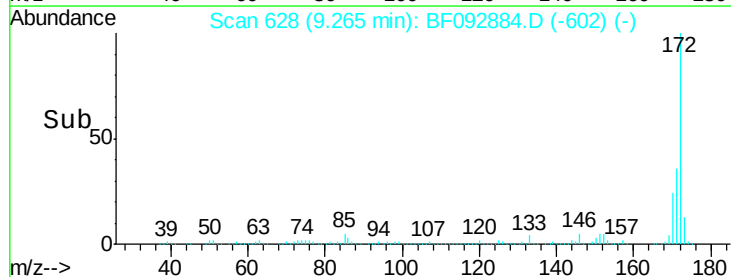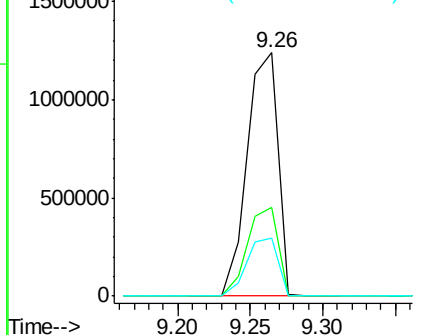


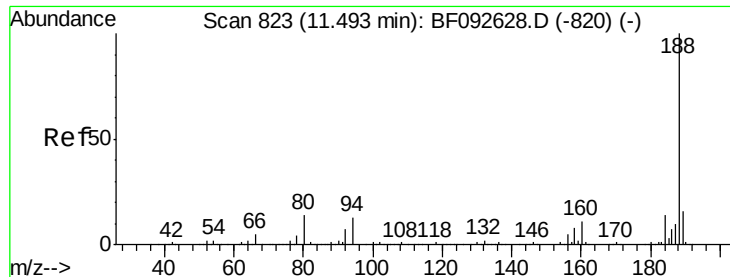




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.42 min Scan# 817
Delta R.T. 0.00 min
Lab File: BF092884.D
Acq: 10 Feb 2017 15:51

Instrument :
BNA_F
ClientSampleId :
PB96853BL

Tgt Ion:188 Resp: 733104
Ion Ratio Lower Upper
188 100
94 8.2 10.0 15.0#
80 8.4 11.2 16.8#

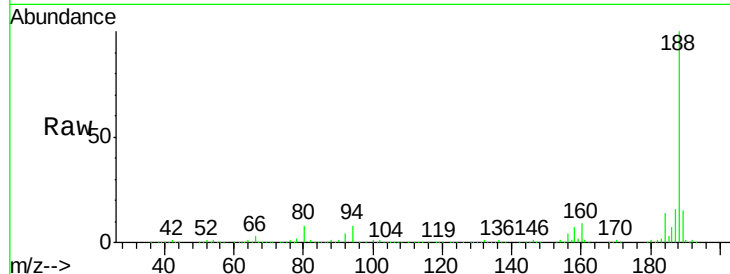


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

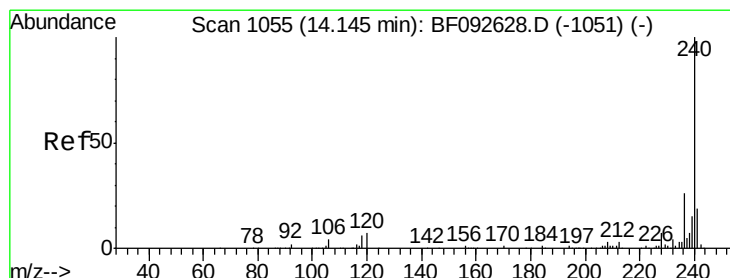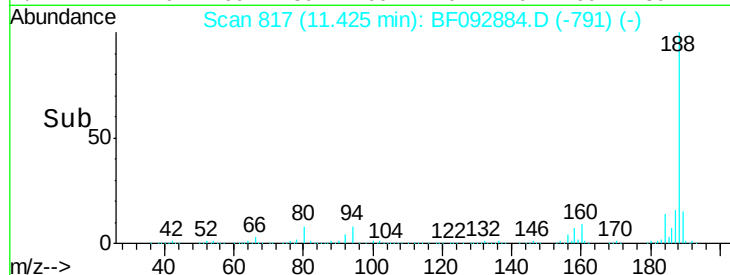
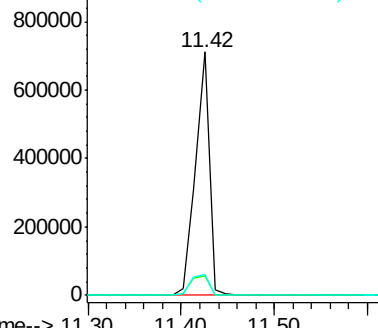



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.05 min Scan# 1047
Delta R.T. -0.01 min
Lab File: BF092884.D
Acq: 10 Feb 2017 15:51

Tgt Ion:240 Resp: 604247
Ion Ratio Lower Upper
240 100
120 17.2 12.9 19.3
236 26.1 20.9 31.3

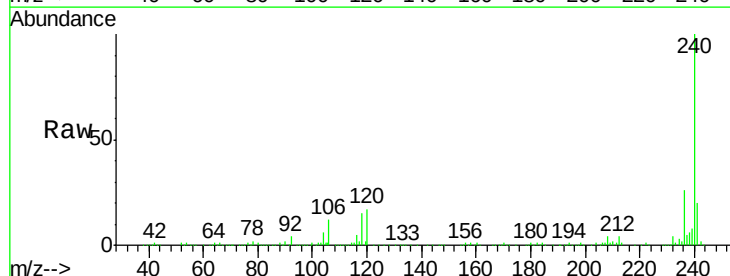

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



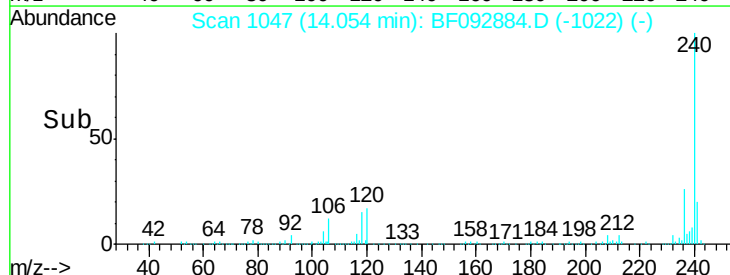
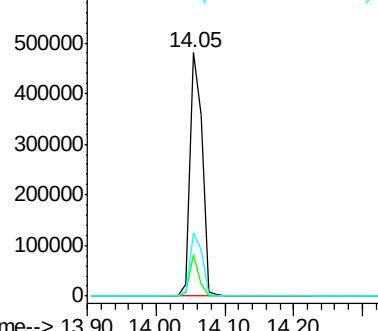


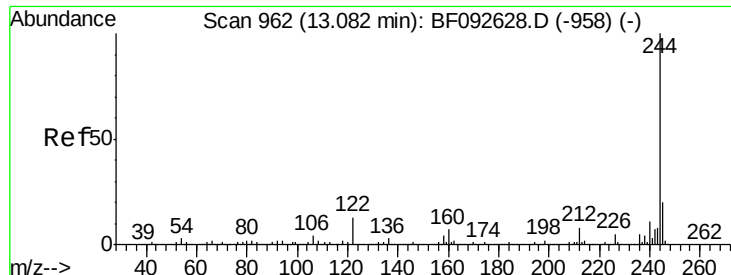

#78
 Terphenyl-d14
 Concen: 63.67 ng
 RT: 13.01 min Scan# 956
 Delta R.T. 0.00 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Instrument :
 BNA_F
 ClientSampleId :
 PB96853BL

Tgt Ion:244 Resp: 1637345
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.2 9.2
 122 11.4 11.4 17.2#

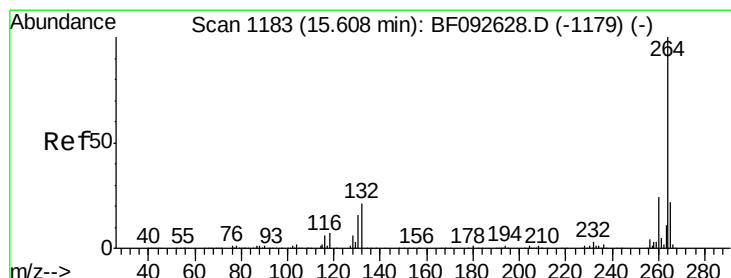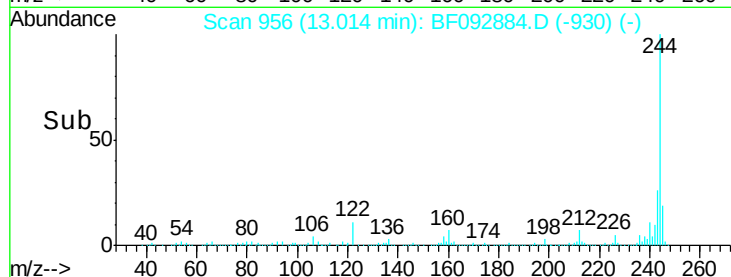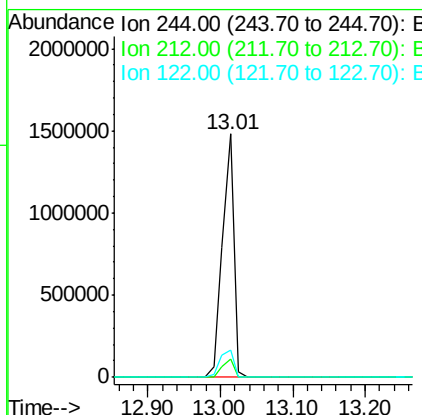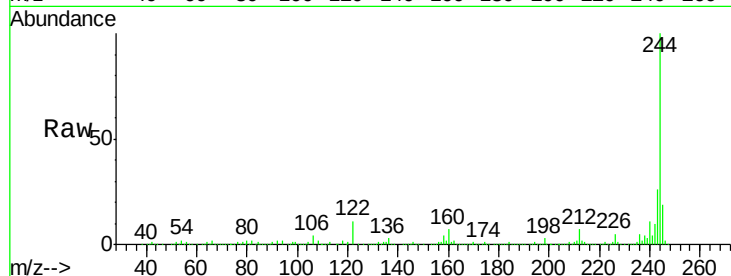

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.51 min Scan# 1174
 Delta R.T. 0.00 min
 Lab File: BF092884.D
 Acq: 10 Feb 2017 15:51

Tgt Ion:264 Resp: 510407
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.2 28.8
 265 21.6 17.4 26.0

