


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021017\
 Data File : BF092882.D
 Acq On : 10 Feb 2017 14:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 14:50:05 2017

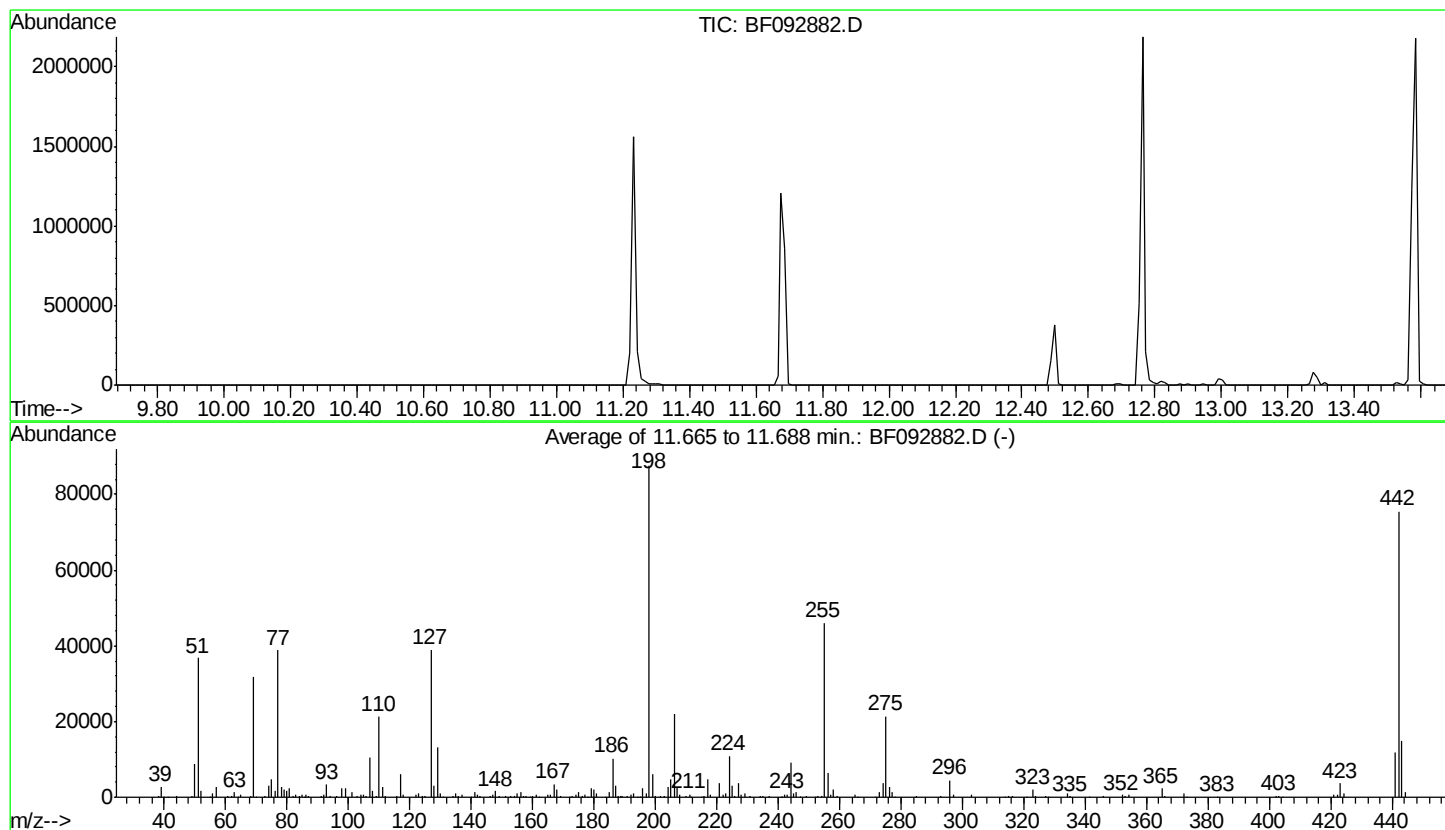

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	36719	PASS
68	69	0.00	2	1.6	499	PASS
69	198	0.00	100	36.2	31740	PASS
70	69	0.00	2	0.4	126	PASS
127	198	10	80	44.5	38956	PASS
197	198	0.00	2	1.2	1054	PASS
198	198	100	100	100.0	87602	PASS
199	198	5	9	6.9	6016	PASS
275	198	10	60	24.4	21398	PASS
365	198	1	100	2.6	2317	PASS
441	442	0.01	24	15.8	11966	PASS
442	198	50	100	86.2	75546	PASS
443	442	15	24	19.6	14784	PASS