
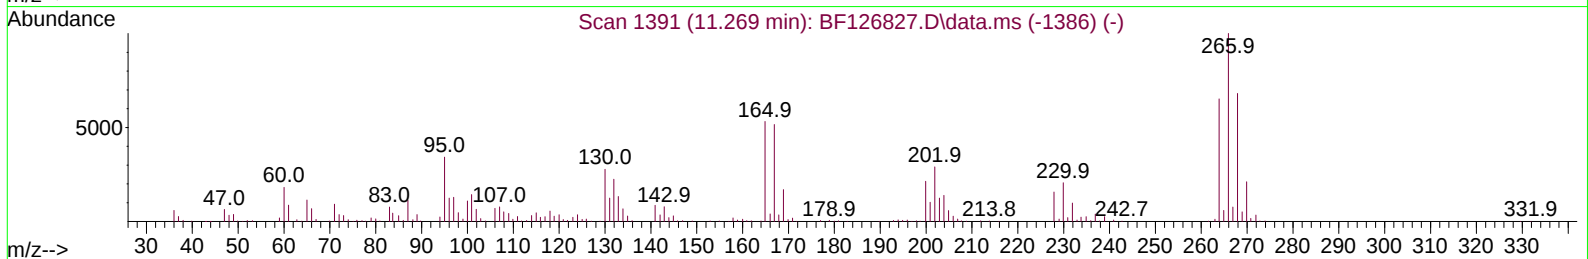
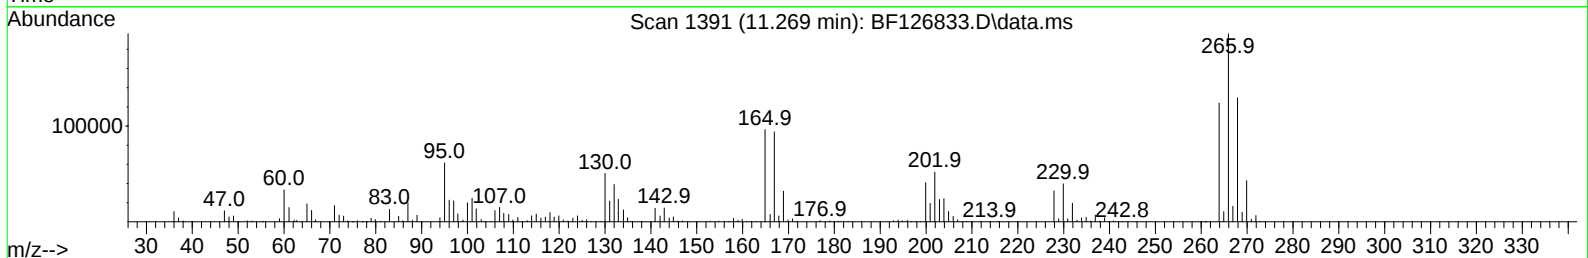


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
 Data File : BF126833.D
 Acq On : 10 Feb 2022 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 12:42:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 10 00:44:00 2022
 Response via : Initial Calibration

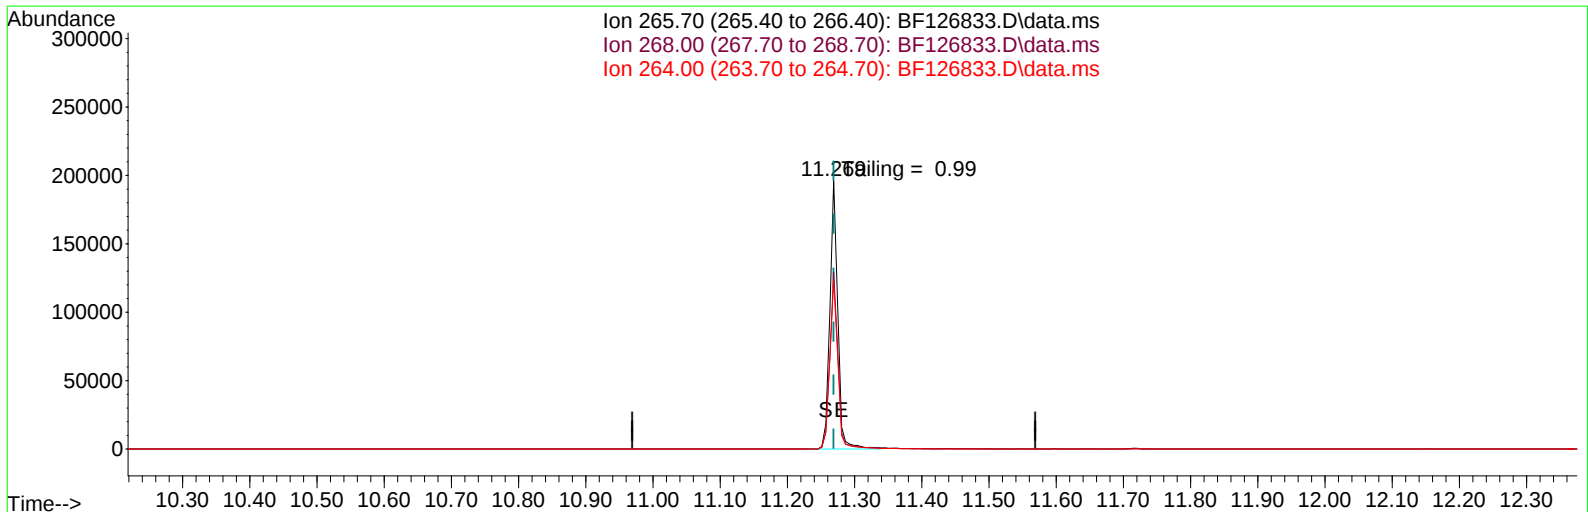

TIC: BF126833.D\data.ms

(70) Pentachlorophenol (C)




11.269min (+ 0.000) 441640.24 ng

response 162713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	65.93
264.00	65.20	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
Data File : BF126833.D
Acq On : 10 Feb 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 12:42:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

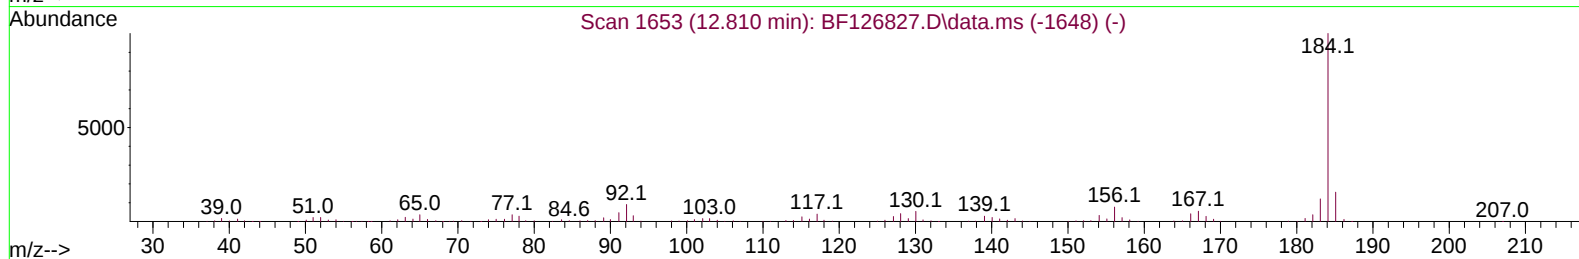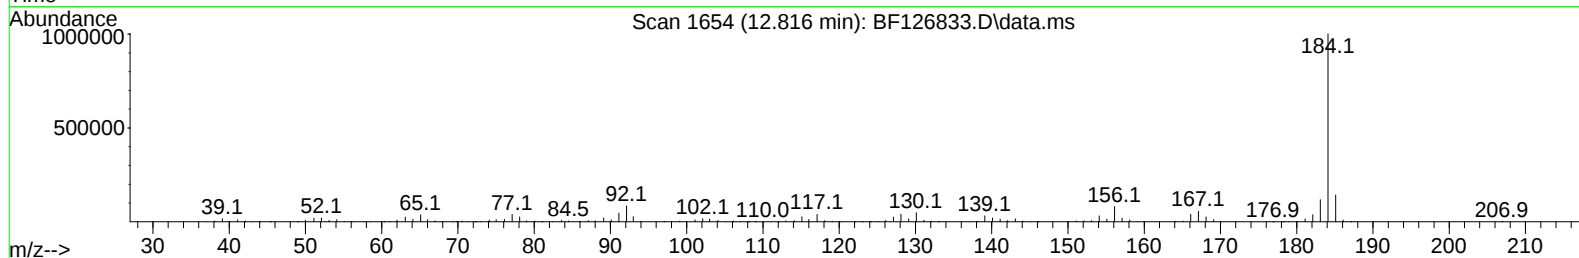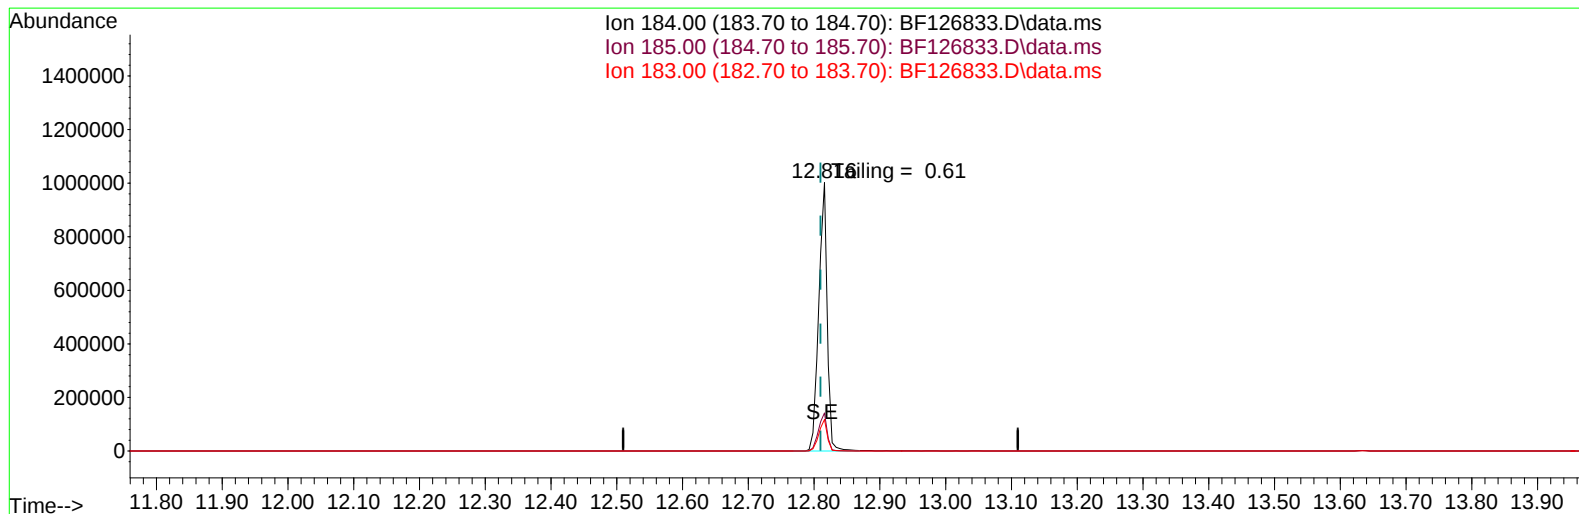

TIC: BF126833.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 11566.09 ng

response 904818

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.21
183.00	12.00	11.75
0.00	0.00	0.00