

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
 Data File : BF126837.D
 Acq On : 10 Feb 2022 12:11
 Operator : CG\JU
 Sample : N1400-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KTS1-WC-S-MH-01-02-0-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.781	110	118	124	rBV	448727	586806	12.52%	1.826%
2	3.869	127	133	138	rVB	39966	50674	1.08%	0.158%
3	4.593	250	256	260	rBV	1786324	1974376	42.13%	6.145%
4	4.775	280	287	292	rBV	410971	439591	9.38%	1.368%
5	4.834	292	297	304	rVB2	154644	177108	3.78%	0.551%
6	5.198	353	359	366	rBV2	436730	580804	12.39%	1.808%
7	5.569	417	422	425	rBV	3226043	3560445	75.98%	11.082%
8	6.563	585	591	594	rBV	2964137	3248537	69.32%	10.111%
9	6.939	652	655	659	rVB	908224	707444	15.10%	2.202%
10	7.228	700	704	707	rBV	120080	96040	2.05%	0.299%
11	7.422	733	737	740	rBV	282547	204079	4.35%	0.635%
12	7.504	745	751	754	rBV	2738300	2720370	58.05%	8.467%
13	7.569	756	762	765	rVV	68117	80965	1.73%	0.252%
14	7.651	773	776	778	rBV	54428	47744	1.02%	0.149%
15	8.222	869	873	876	rBV	1179965	951048	20.30%	2.960%
16	8.486	916	918	922	rVB	140875	108259	2.31%	0.337%
17	9.139	1024	1029	1032	rBV3	84290	152305	3.25%	0.474%
18	9.175	1032	1035	1042	rVB	187507	269351	5.75%	0.838%
19	9.298	1051	1056	1059	rBV	4868240	4315525	92.09%	13.432%
20	9.422	1074	1077	1082	rBV2	64562	99371	2.12%	0.309%
21	9.469	1082	1085	1087	rVV	64483	72943	1.56%	0.227%
22	9.498	1087	1090	1098	rVB	81469	106709	2.28%	0.332%
23	9.686	1119	1122	1124	rBV	65366	48026	1.02%	0.149%
24	9.710	1124	1126	1129	rVB	150451	126454	2.70%	0.394%
25	9.980	1168	1172	1175	rVB	1059719	931330	19.87%	2.899%
26	10.051	1181	1184	1186	rBV	64503	53710	1.15%	0.167%
27	10.769	1301	1306	1310	rBV	2876587	3009796	64.23%	9.368%
28	11.469	1421	1425	1429	rBV	1338321	1090059	23.26%	3.393%
29	11.986	1509	1513	1517	rBV2	57782	75890	1.62%	0.236%
30	13.063	1691	1696	1699	rBV	4929406	4686111	100.00%	14.585%
31	13.533	1770	1776	1785	rBV2	46565	99740	2.13%	0.310%
32	13.974	1848	1851	1856	rVB	43640	47498	1.01%	0.148%
33	14.115	1871	1875	1878	rBV	781897	748194	15.97%	2.329%
34	14.210	1885	1891	1897	rVB	56879	84628	1.81%	0.263%
35	14.292	1902	1905	1908	rBV	103773	91292	1.95%	0.284%
36	14.757	1978	1984	1988	rBV	62298	102415	2.19%	0.319%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
Data File : BF126837.D
Acq On : 10 Feb 2022 12:11
Operator : CG\JU
Sample : N1400-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.804	1988	1992	2002	rVB8	38157	72523	1.55%	0.226%
38	15.351	2080	2085	2092	rVB	38169	68569	1.46%	0.213%
39	15.621	2126	2131	2138	rBV2	112993	169889	3.63%	0.529%
40	16.033	2194	2201	2209	rBV5	29927	72369	1.54%	0.225%




Sum of corrected areas: 32128987

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
Data File : BF126837.D
Acq On : 10 Feb 2022 12:11
Operator : CG\JU
Sample : N1400-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

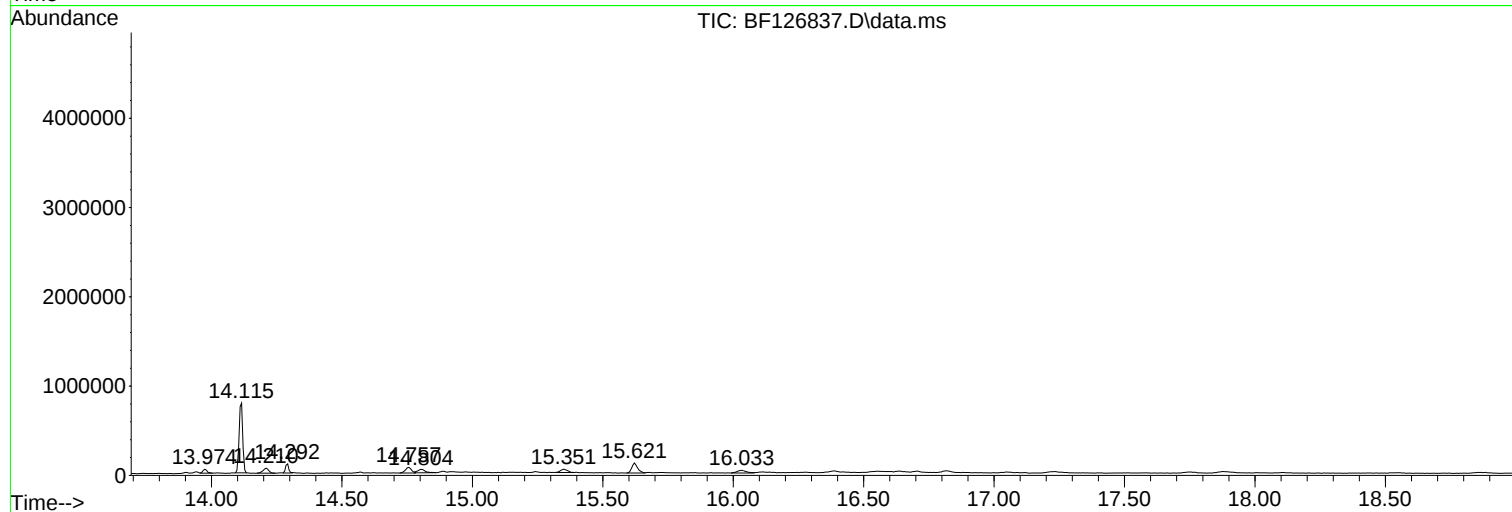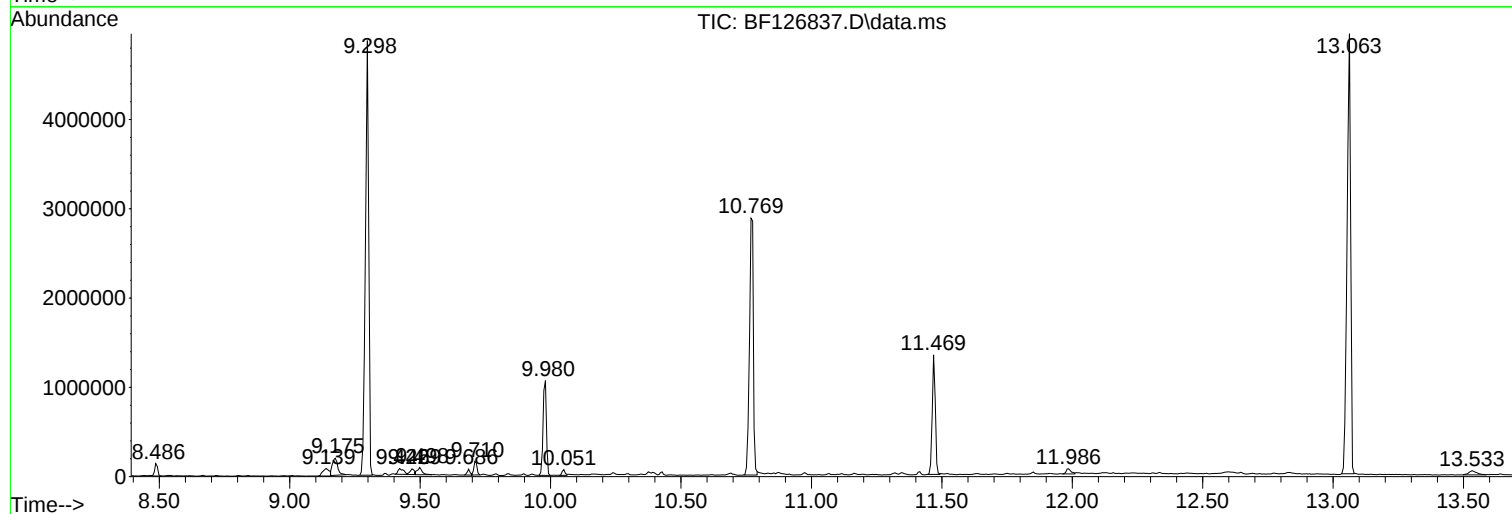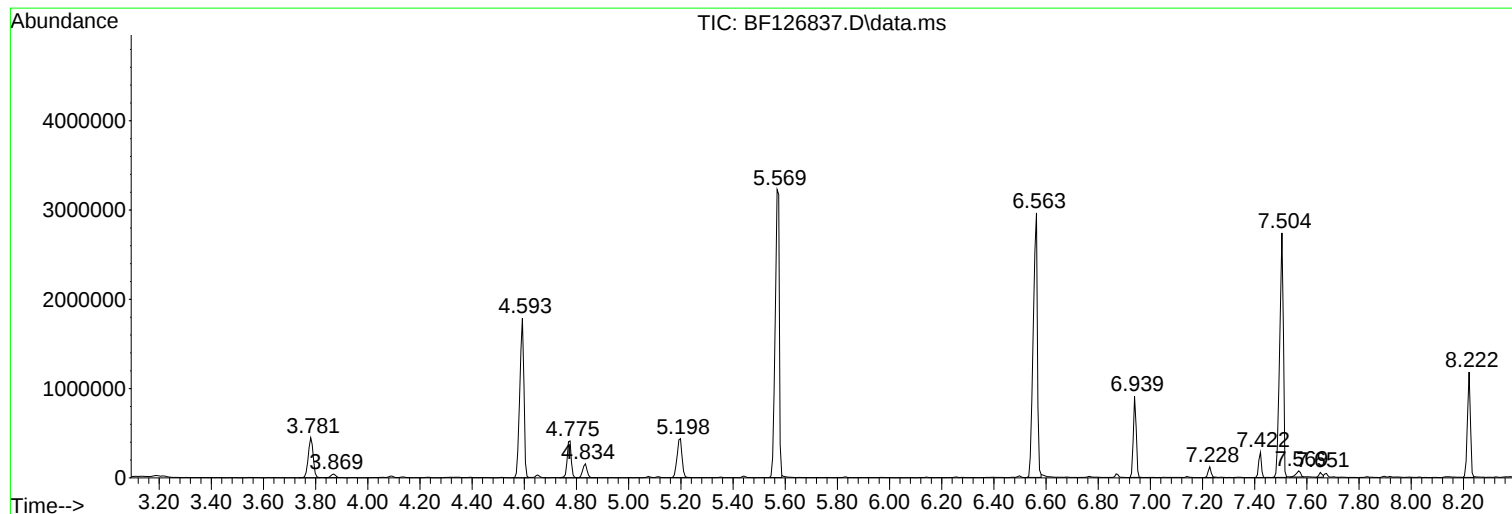

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
Data File : BF126837.D
Acq On : 10 Feb 2022 12:11
Operator : CG\JU
Sample : N1400-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021022\
Data File : BF126837.D
Acq On : 10 Feb 2022 12:11
Operator : CG\JU
Sample : N1400-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KTS1-WC-S-MH-01-02-0-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------