


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021022\  
 Data File : BF126833.D  
 Acq On : 10 Feb 2022 10:08  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Feb 10 00:44:00 2022

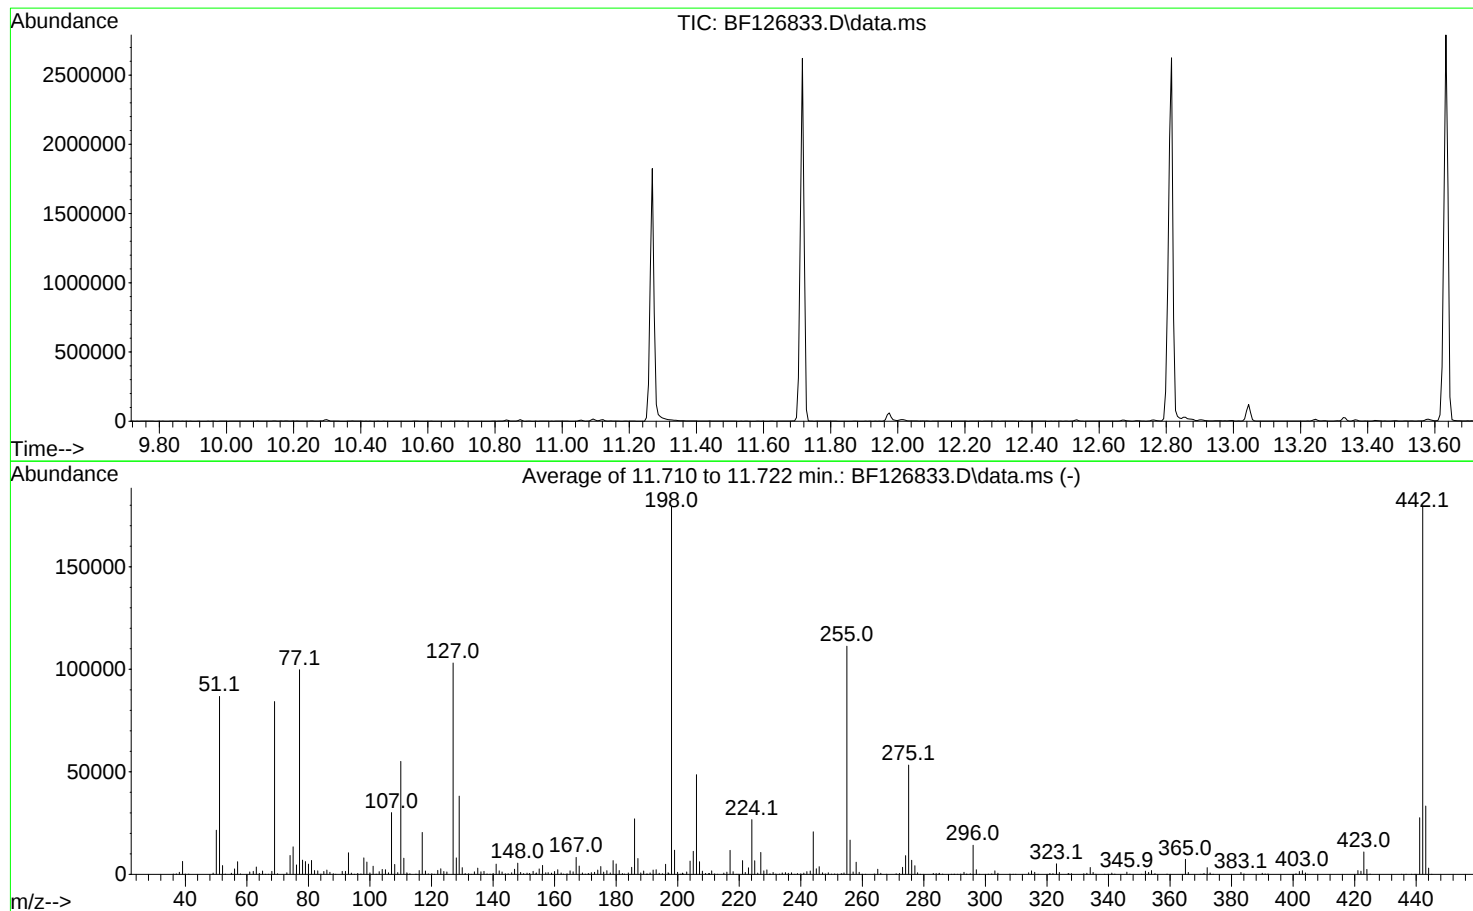




AutoFind: Scans 1466, 1467, 1468; Background Corrected with Scan 1460

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 48.4         | 86779      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1482       | PASS                |
| 69             | 198             | 0.00            | 100             | 47.0         | 84299      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 355        | PASS                |
| 127            | 198             | 10              | 80              | 57.5         | 103085     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 767        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 179203     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 11793      | PASS                |
| 275            | 198             | 10              | 60              | 29.7         | 53288      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 7330       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.4         | 27652      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 179392     | PASS                |
| 443            | 442             | 15              | 24              | 18.6         | 33288      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021022\  
 Data File : BF126833.D  
 Acq On : 10 Feb 2022 10:08  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 10 12:42:26 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Feb 10 00:44:00 2022  
 Response via : Initial Calibration

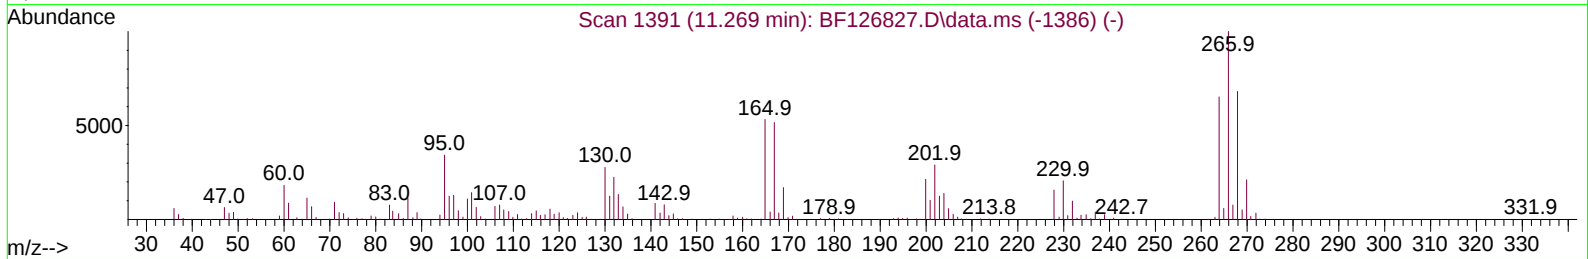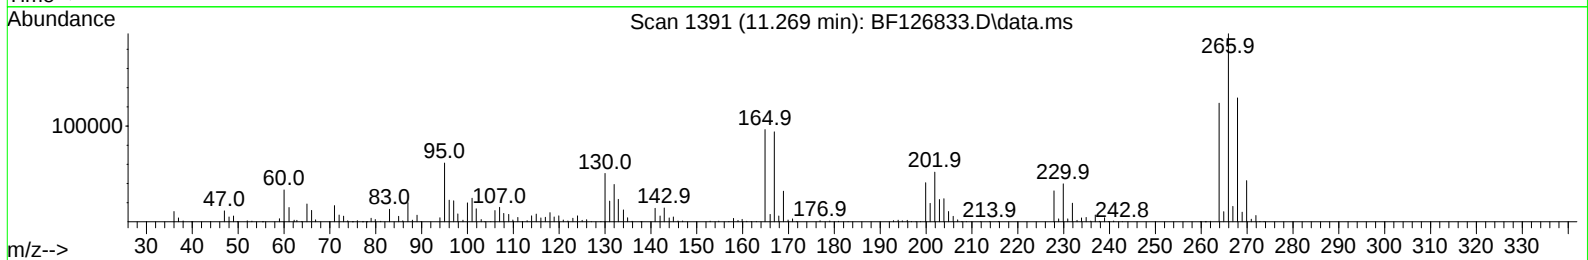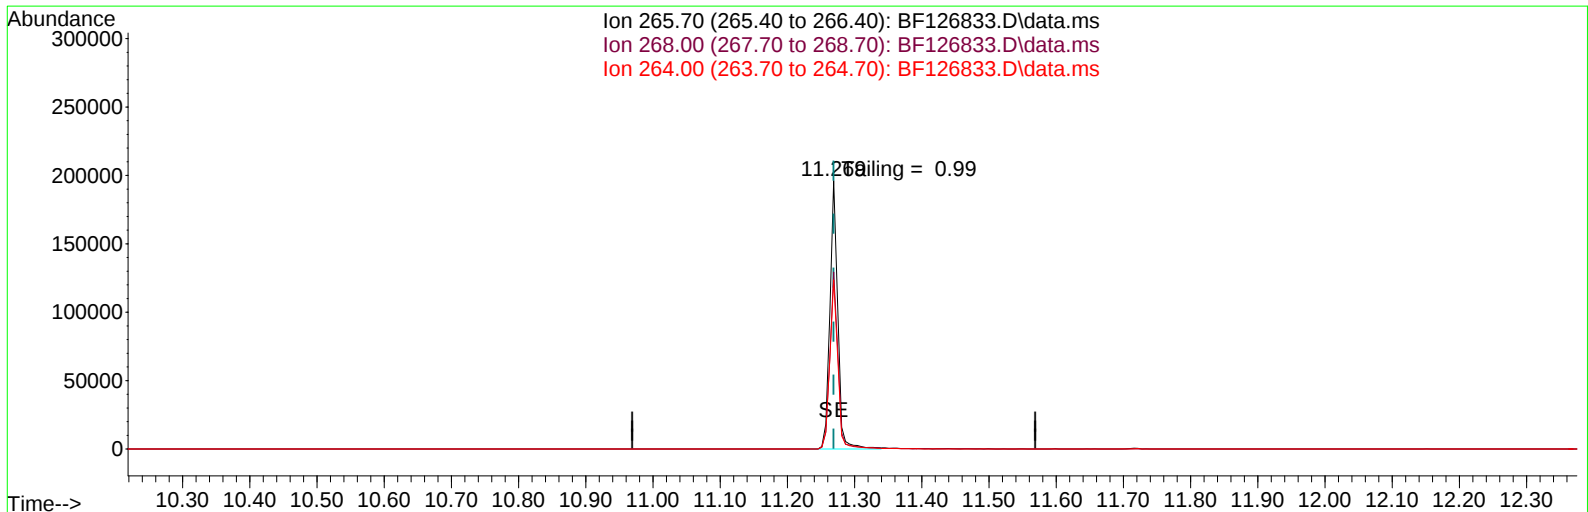

TIC: BF126833.D\data.ms

**(70) Pentachlorophenol (C)**

**11.269min (+ 0.000) 441640.24 ng**




**response 162713**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 68.10  | 65.93  |
| 264.00 | 65.20  | 63.06  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021022\  
Data File : BF126833.D  
Acq On : 10 Feb 2022 10:08  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Feb 10 12:42:26 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 10 00:44:00 2022  
Response via : Initial Calibration

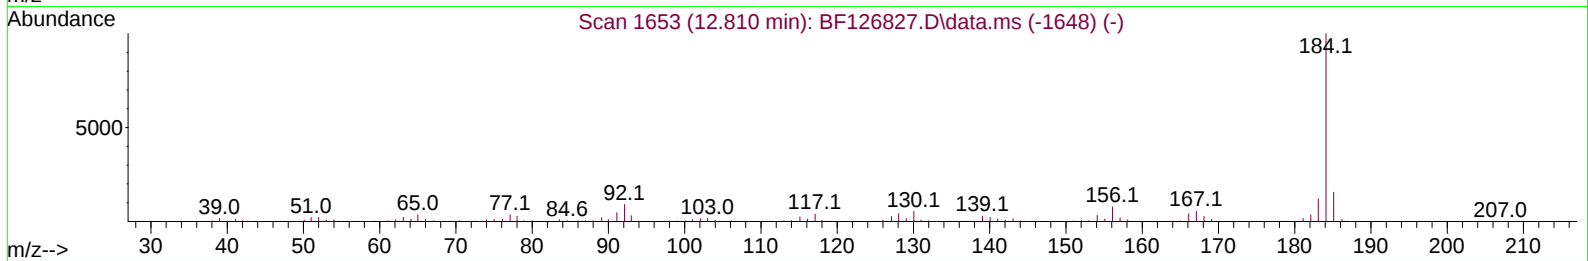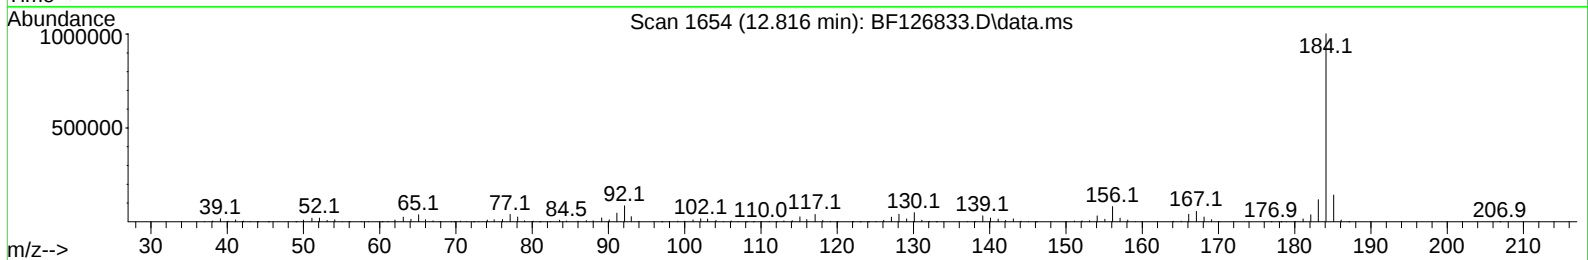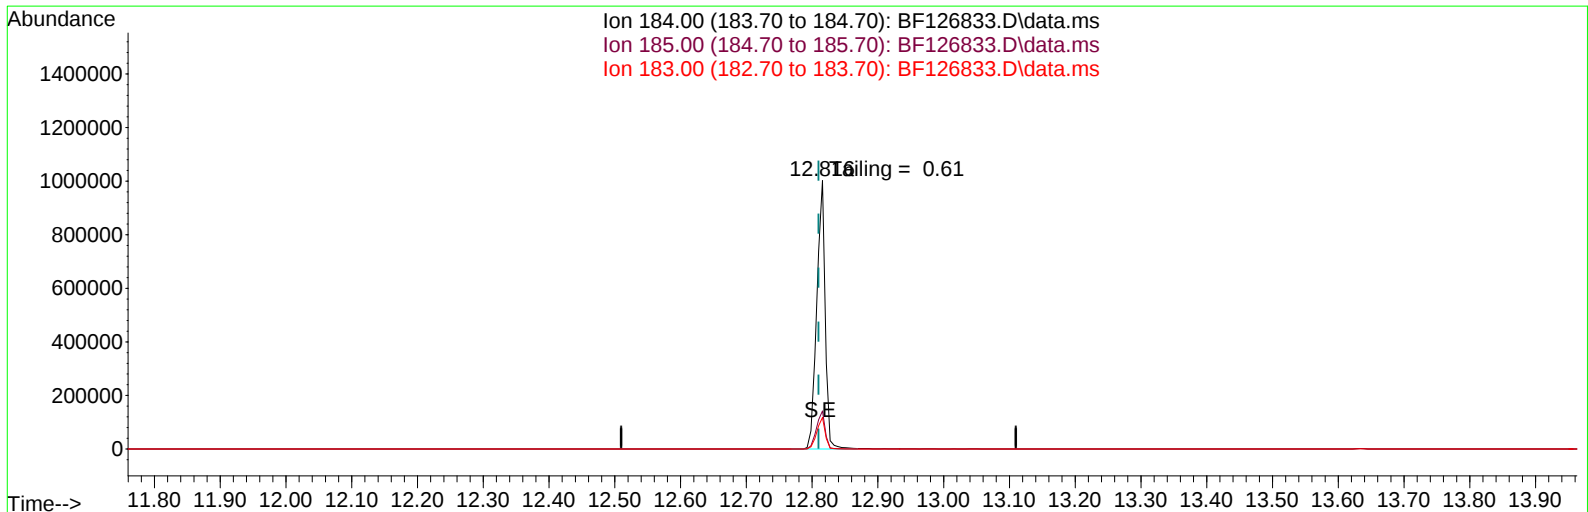

TIC: BF126833.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 11566.09 ng

response 904818

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.60  | 14.21  |
| 183.00 | 12.00  | 11.75  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/10/2022     | BNA_F            | <u>BF126833.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 410742           | 13.63              |
| DDD           | 4124             | 13.33              |
| DDE           | 540              | 13.04              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 4664          | 415406           | 1.12               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP