
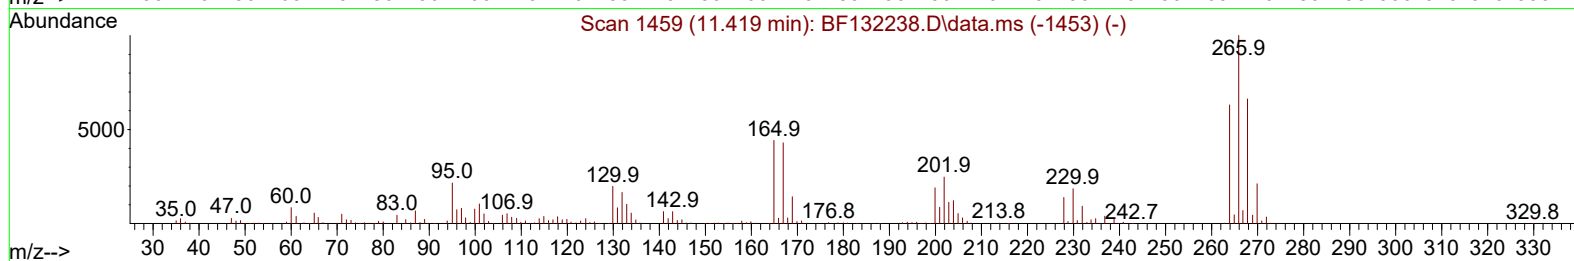
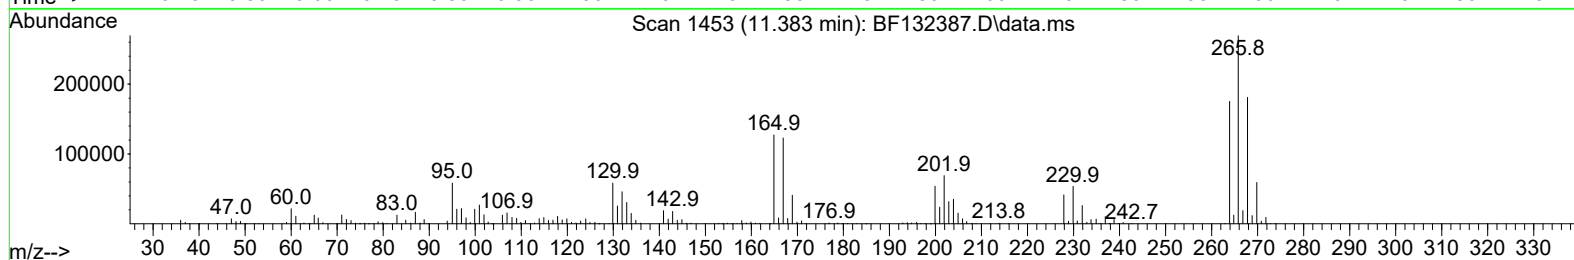


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021023\
Data File : BF132387.D
Acq On : 10 Feb 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 02:50:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 11 00:16:13 2023
Response via : Initial Calibration

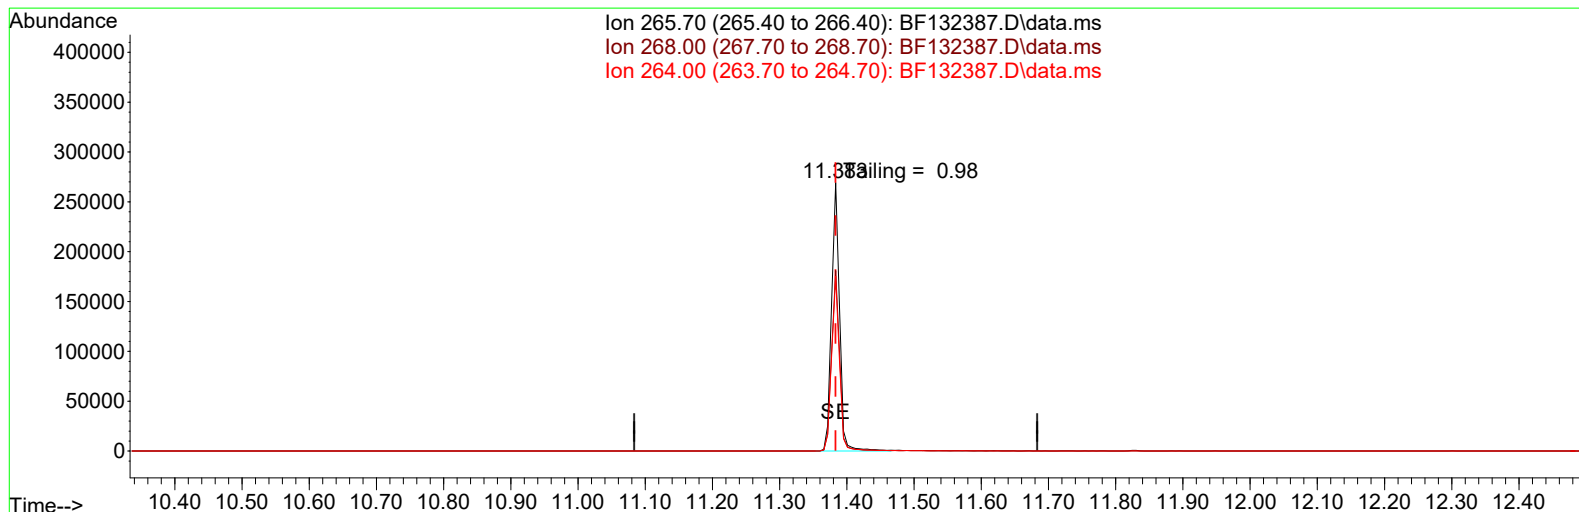

TIC: BF132387.D\data.ms

(70) Pentachlorophenol (C)




11.383min (-0.000) 29301.04 ng

response 225194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	67.22
264.00	63.10	65.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021023\
Data File : BF132387.D
Acq On : 10 Feb 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 02:50:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 11 00:16:13 2023
Response via : Initial Calibration

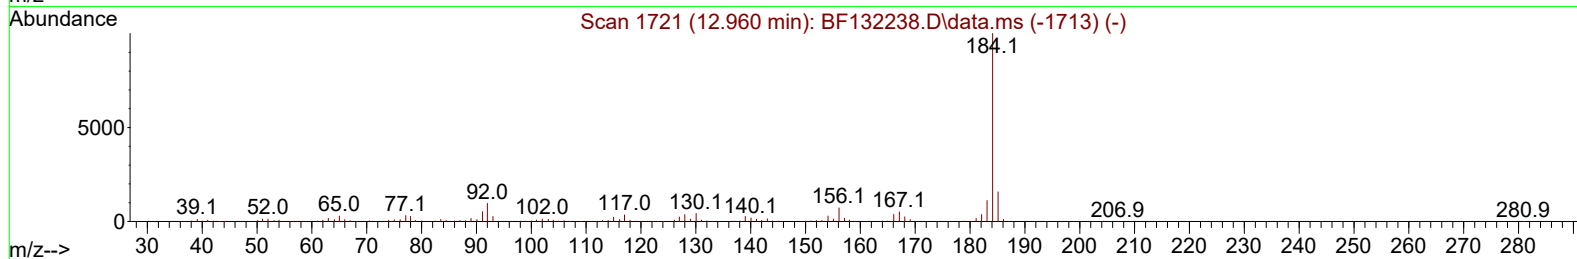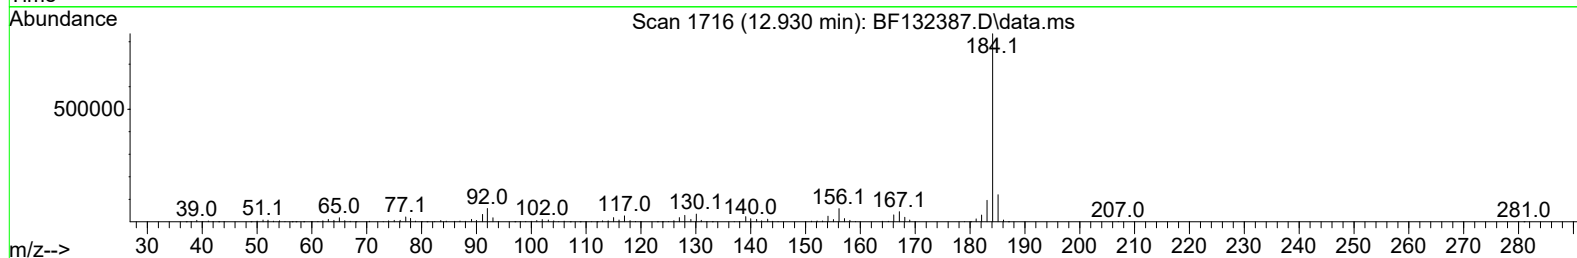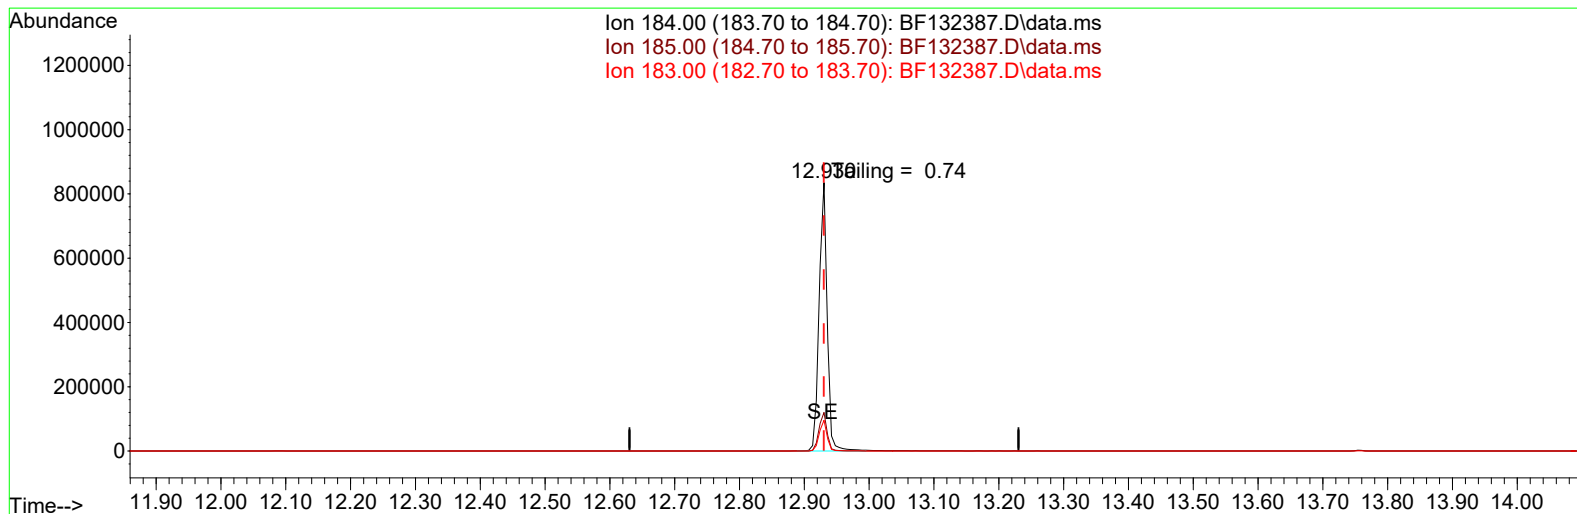

TIC: BF132387.D\data.ms

(77) Benzidine

12.930min (-0.000) 0.00 ng

response 727173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.41
183.00	11.10	11.43
0.00	0.00	0.00