


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021023\
 Data File : BF132387.D
 Acq On : 10 Feb 2023 11:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 11 00:16:13 2023

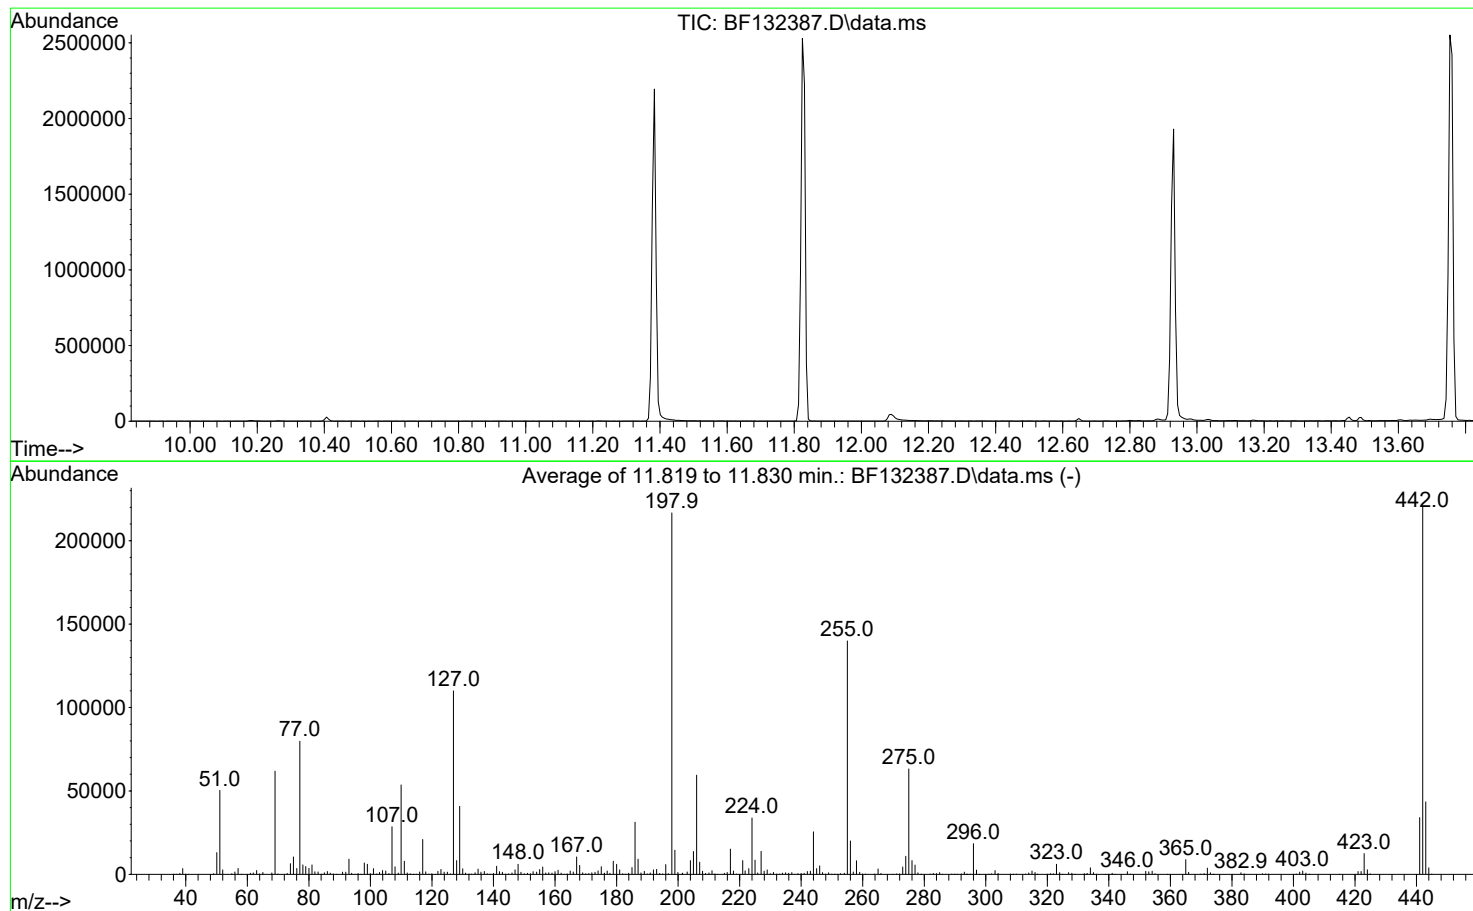

AutoFind: Scans 1527, 1528, 1529; Background Corrected with Scan 1522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	50349	PASS
68	69	0.00	2	1.5	918	PASS
69	198	0.00	100	28.6	61864	PASS
70	69	0.00	2	0.6	342	PASS
127	198	10	80	50.8	109995	PASS
197	198	0.00	2	0.2	414	PASS
198	198	100	100	100.0	216619	PASS
199	198	5	9	6.7	14469	PASS
275	198	10	60	29.2	63227	PASS
365	198	1	100	4.1	8852	PASS
441	198	0.01	100	15.7	34102	PASS
442	442	50	100	100.0	220491	PASS
443	442	15	24	19.7	43464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/10/2023	BNA_F	<u>BF132387.D</u>
Compound Name	Response	Retention Time
DDT	733768	13.76
DDD	8304	13.454
DDE	520	13.113
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8824	742592	1.19

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021023\
 Data File : BF132387.D
 Acq On : 10 Feb 2023 11:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 11 02:50:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 11 00:16:13 2023
 Response via : Initial Calibration

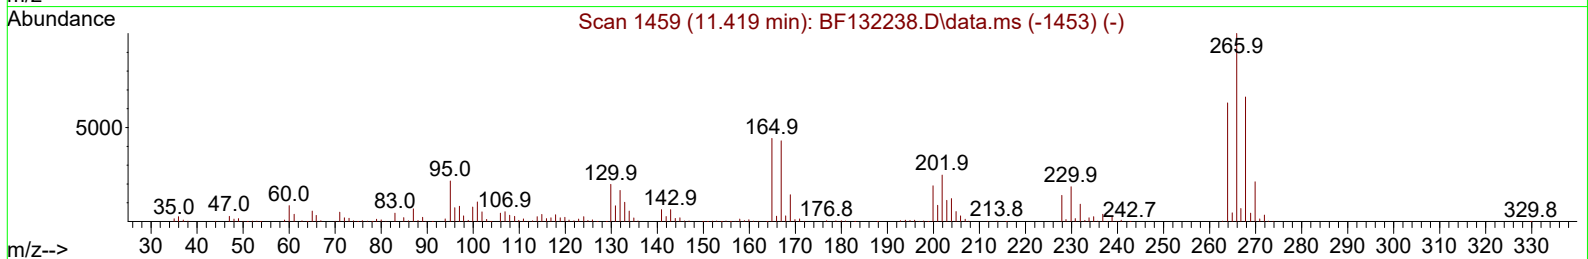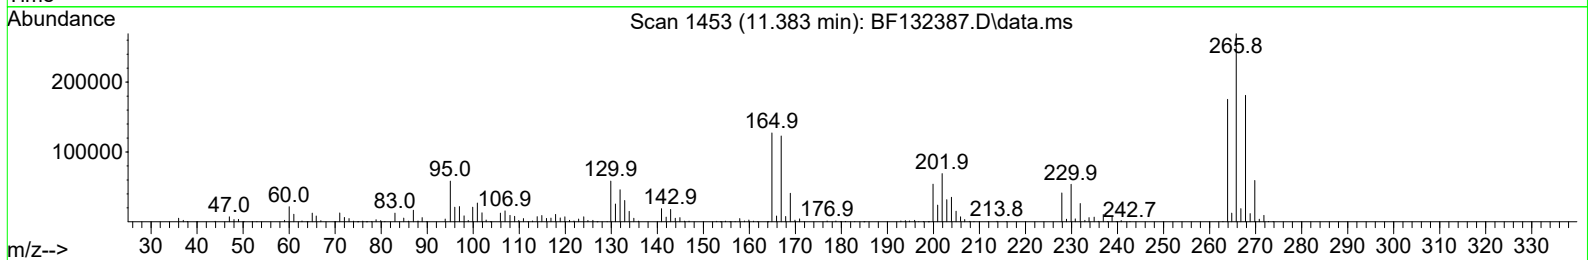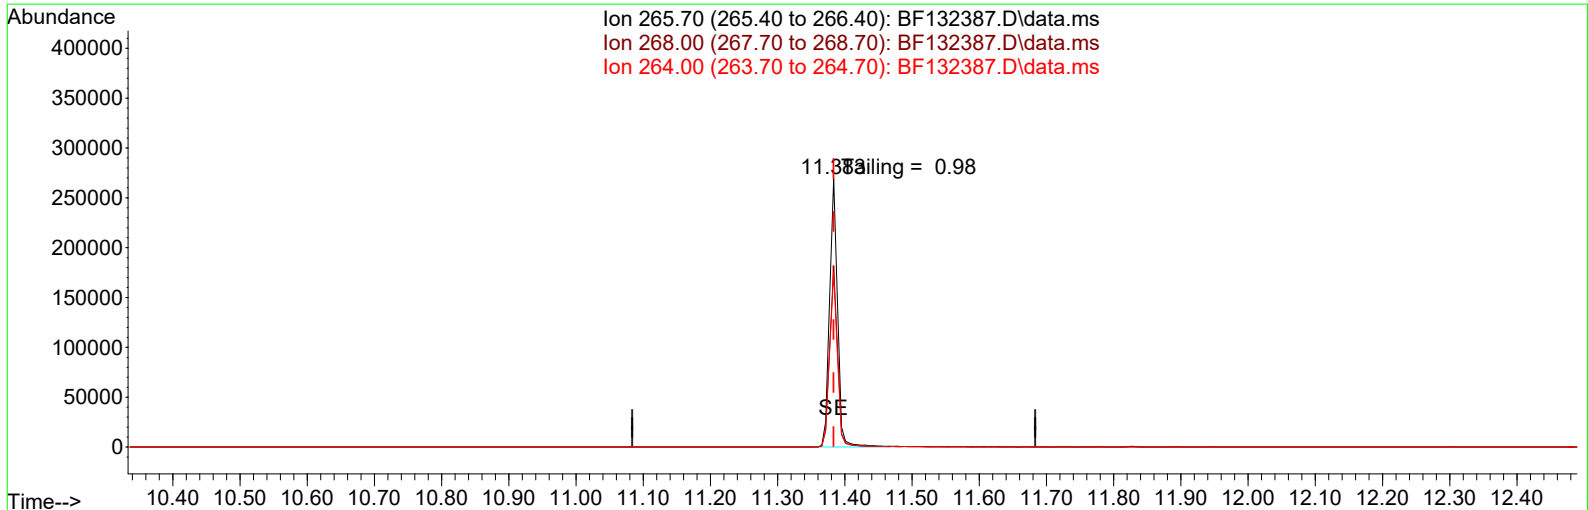

TIC: BF132387.D\data.ms

(70) Pentachlorophenol (C)

11.383min (-0.000) 29301.04 ng




response 225194

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	67.22
264.00	63.10	65.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021023\
Data File : BF132387.D
Acq On : 10 Feb 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 11 02:50:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF013123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 11 00:16:13 2023
Response via : Initial Calibration

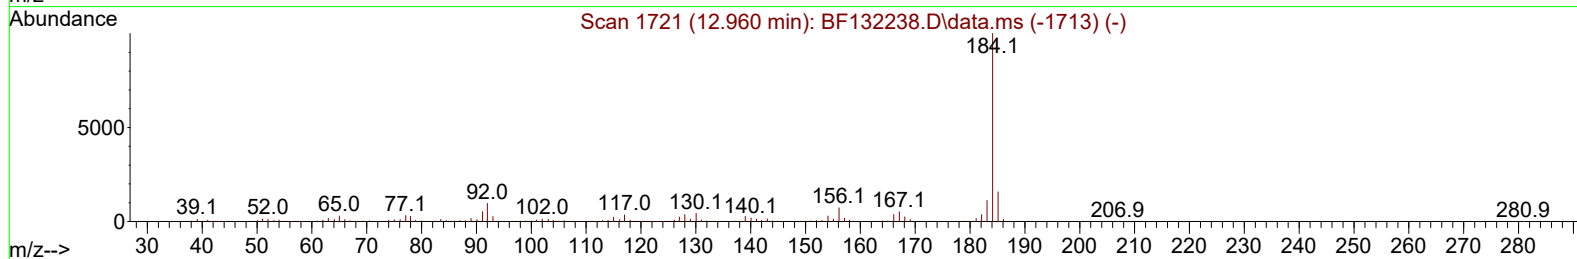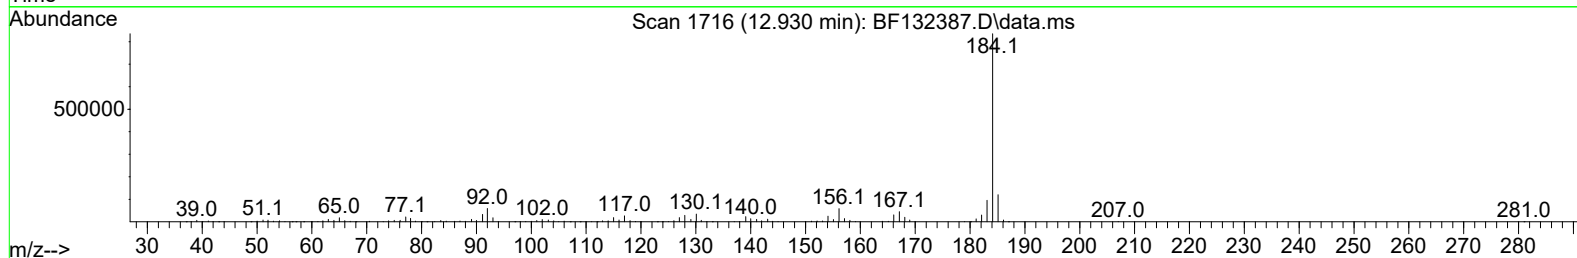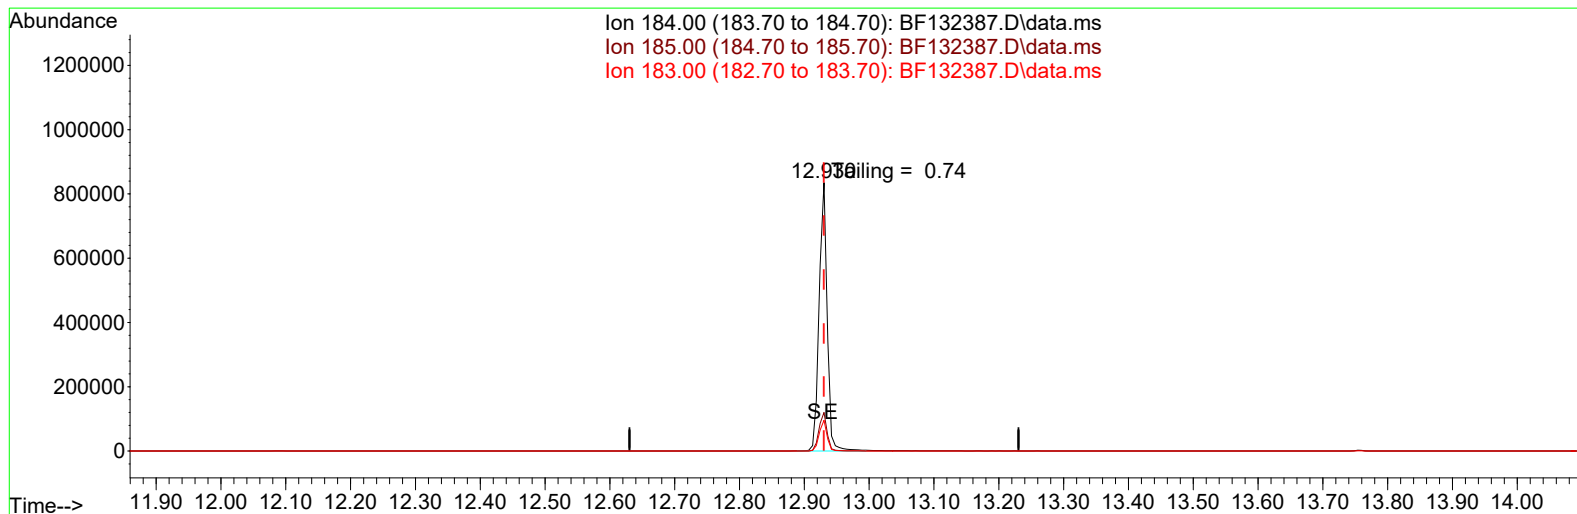

TIC: BF132387.D\data.ms

(77) Benzidine

12.930min (-0.000) 0.00 ng

response 727173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.41
183.00	11.10	11.43
0.00	0.00	0.00