

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
 Data File : BF141535.D
 Acq On : 10 Feb 2025 15:17
 Operator : RC/JU
 Sample : PB166619BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166619BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.863	293	301	312	rBV	43687	73362	1.66%	0.348%
2	5.416	560	565	587	rBV	1557358	2085501	47.20%	9.892%
3	6.428	731	737	757	rBV	1502846	2085454	47.20%	9.892%
4	6.787	793	798	809	rVB	489491	604483	13.68%	2.867%
5	7.351	887	894	899	rBV	1447490	2073355	46.93%	9.835%
6	8.069	1010	1016	1038	rBV	589245	806010	18.24%	3.823%
7	9.145	1192	1199	1204	rBV	2754276	3791887	85.82%	17.986%
8	9.822	1307	1314	1331	rBV	706987	927708	21.00%	4.400%
9	10.610	1442	1448	1478	rBV	1144312	1587058	35.92%	7.528%
10	11.310	1561	1567	1574	rBV	757430	963778	21.81%	4.571%
11	12.898	1831	1837	1843	rBV	3204000	4418417	100.00%	20.958%
12	13.951	2010	2016	2024	rBV	695608	909034	20.57%	4.312%
13	15.404	2257	2263	2274	rVB	468311	756313	17.12%	3.587%




Sum of corrected areas: 21082360

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141535.D
Acq On : 10 Feb 2025 15:17
Operator : RC/JU
Sample : PB166619BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166619BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

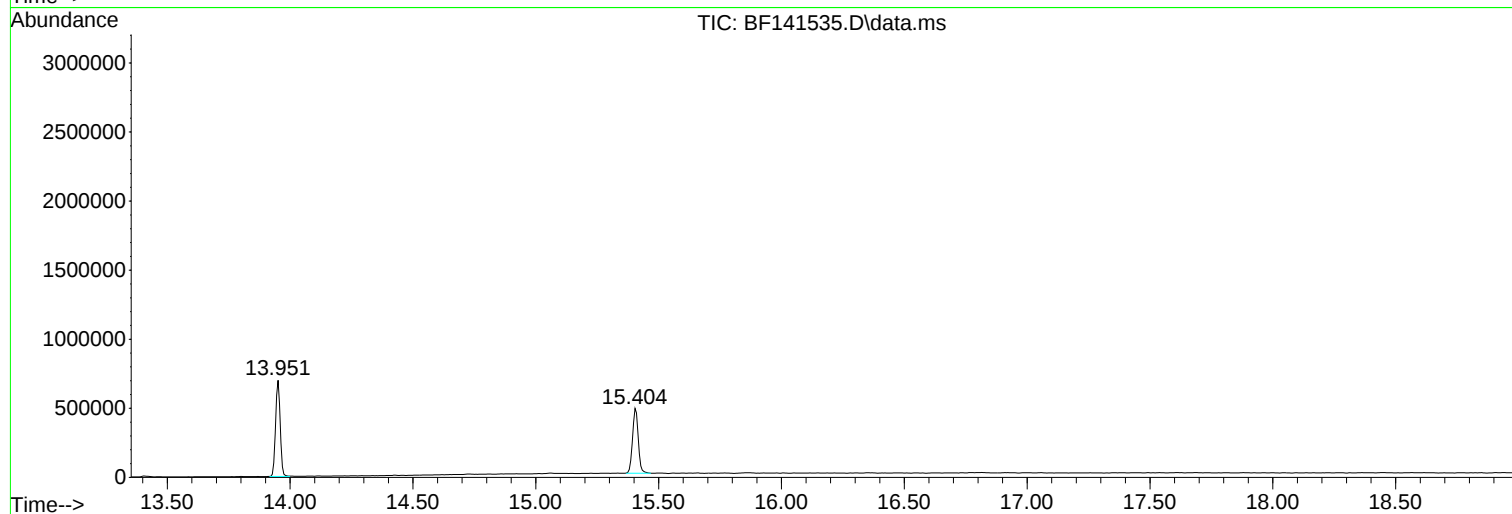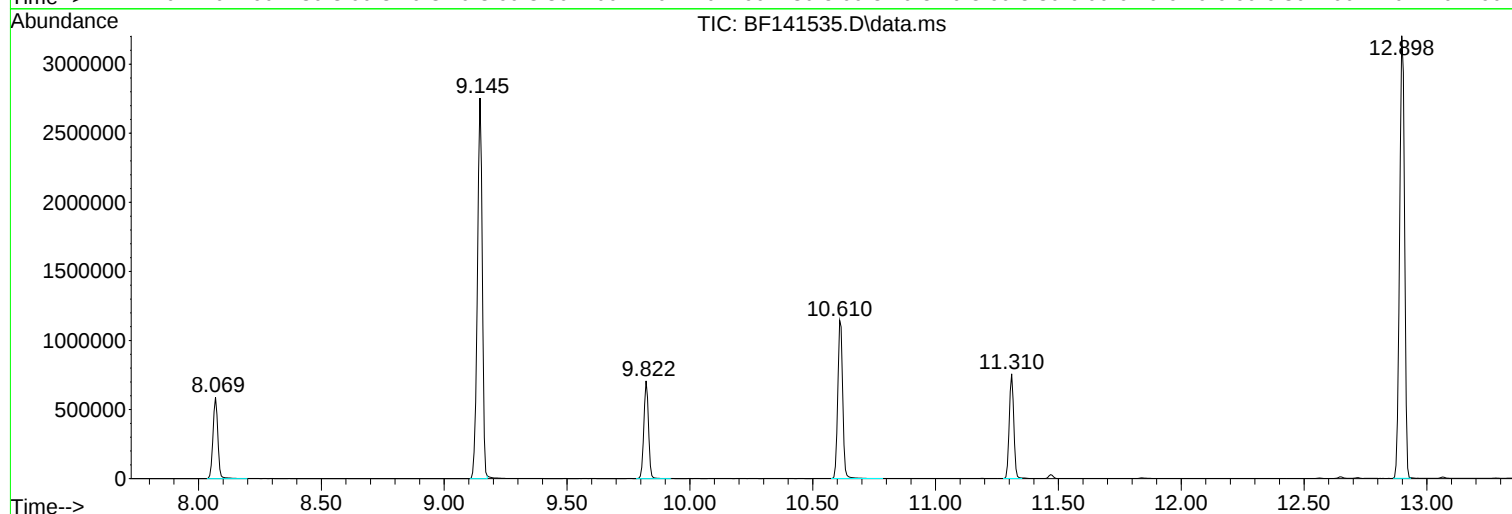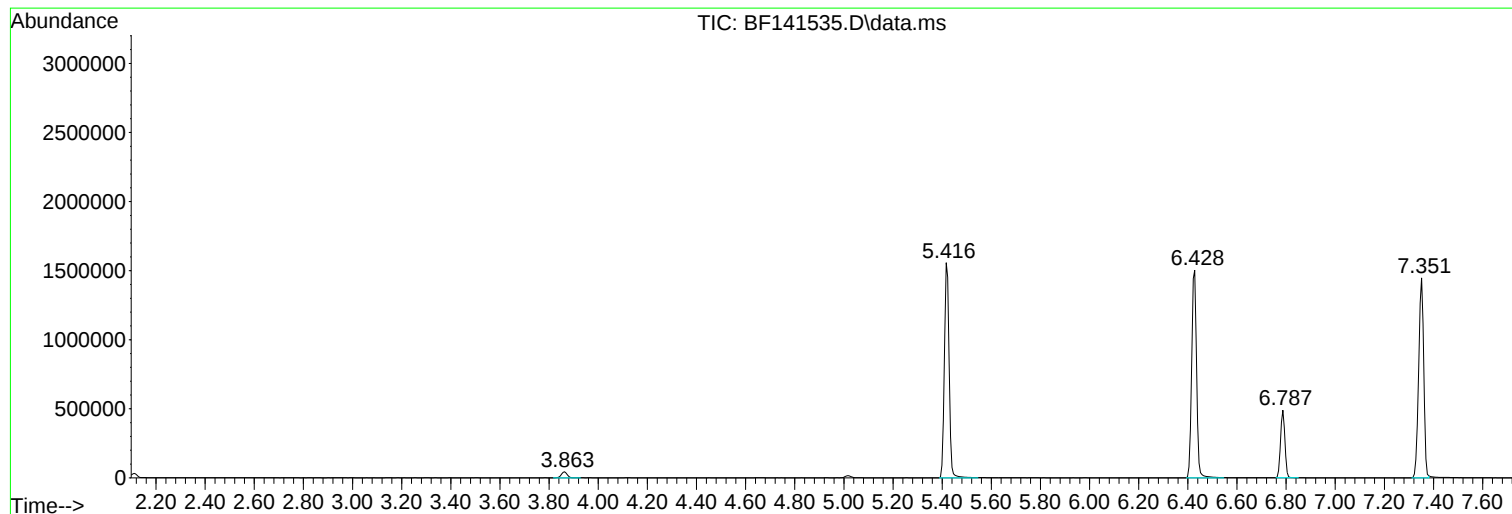

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141535.D
Acq On : 10 Feb 2025 15:17
Operator : RC/JU
Sample : PB166619BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166619BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021025\
Data File : BF141535.D
Acq On : 10 Feb 2025 15:17
Operator : RC/JU
Sample : PB166619BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166619BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------