
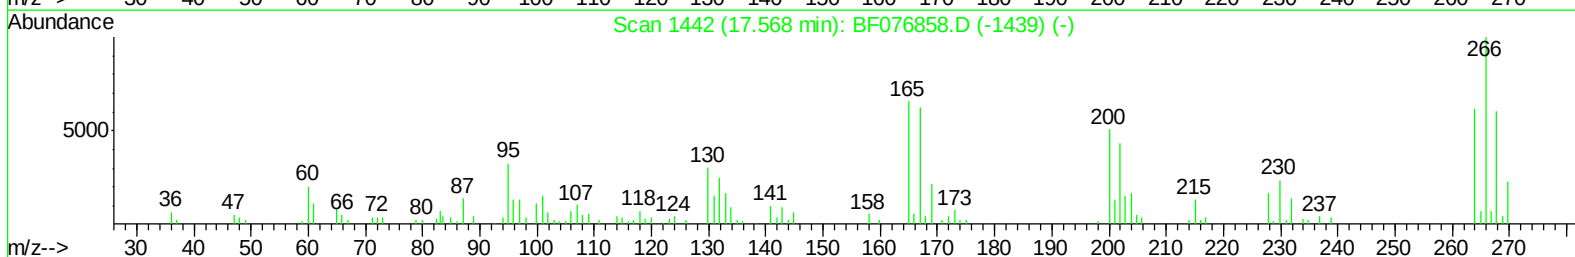
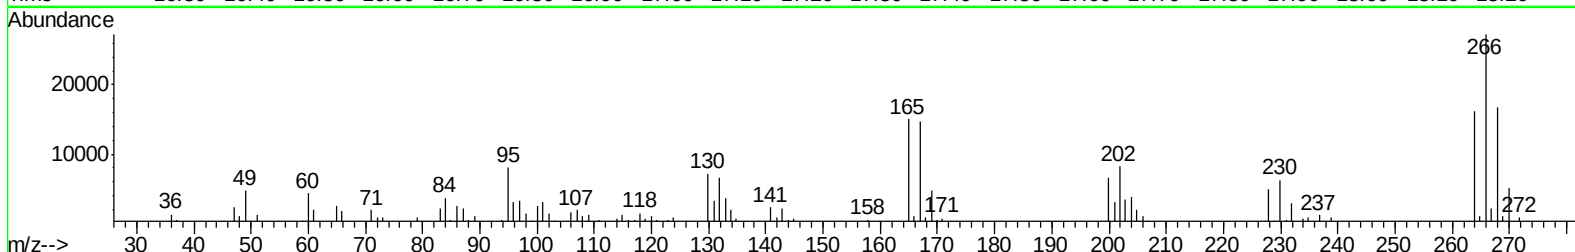


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077249.D
Acq On : 11 Feb 2015 11:59
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 03:38:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

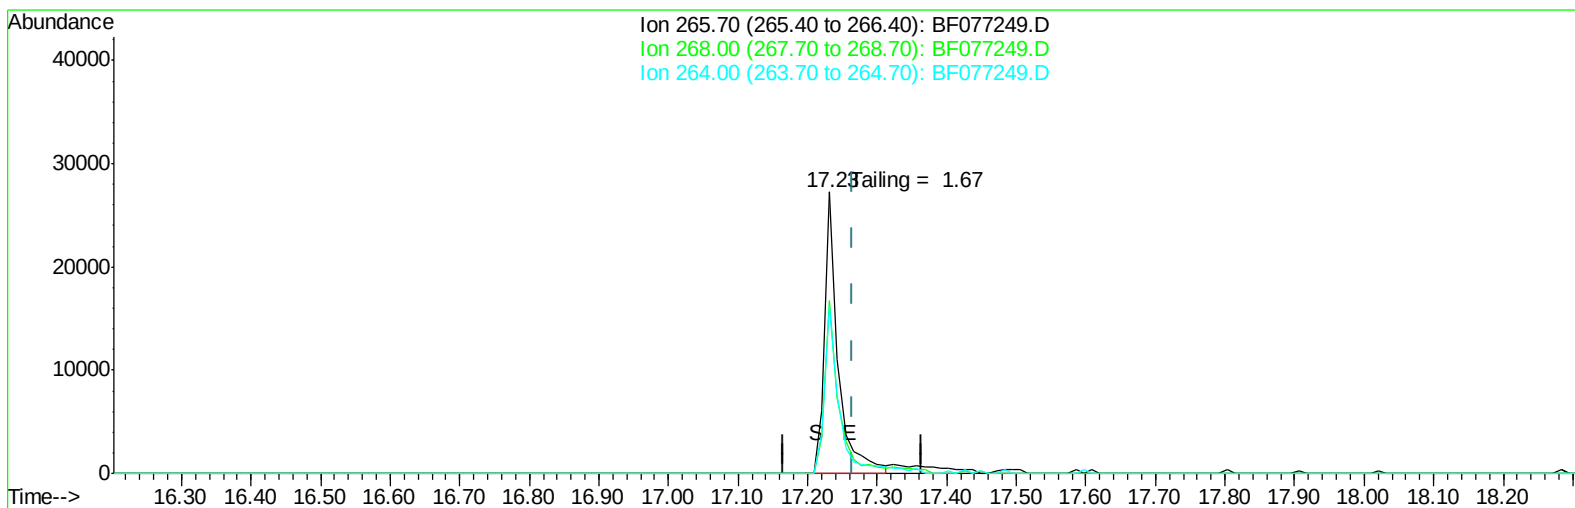

TIC: BF077249.D

(69) Pentachlorophenol (C)




17.231min (-0.034) 0.00ng

response 37474

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.50
264.00	61.90	59.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077249.D
Acq On : 11 Feb 2015 11:59
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 03:38:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

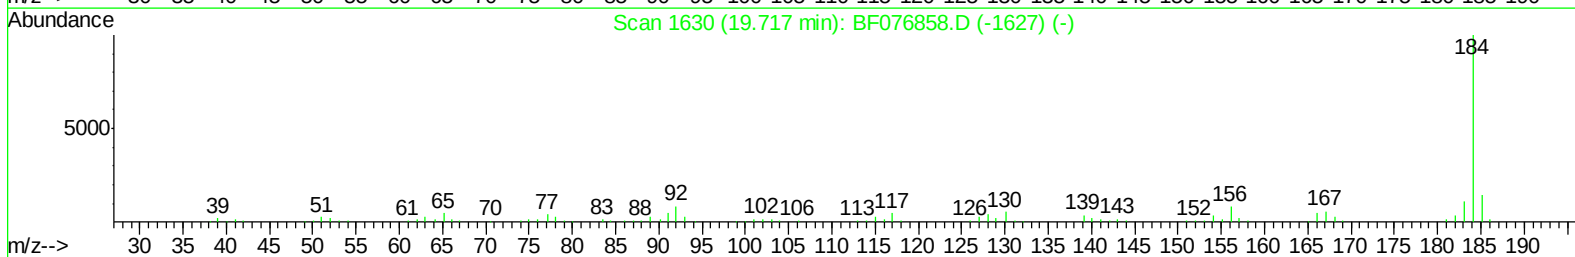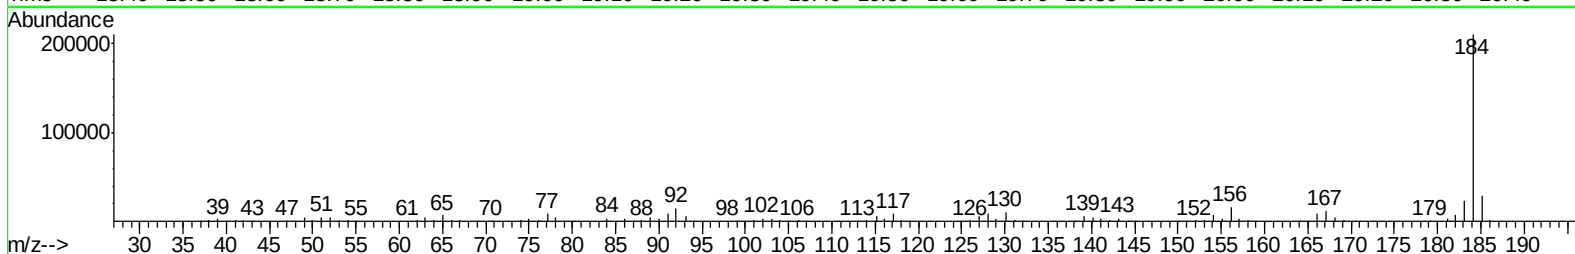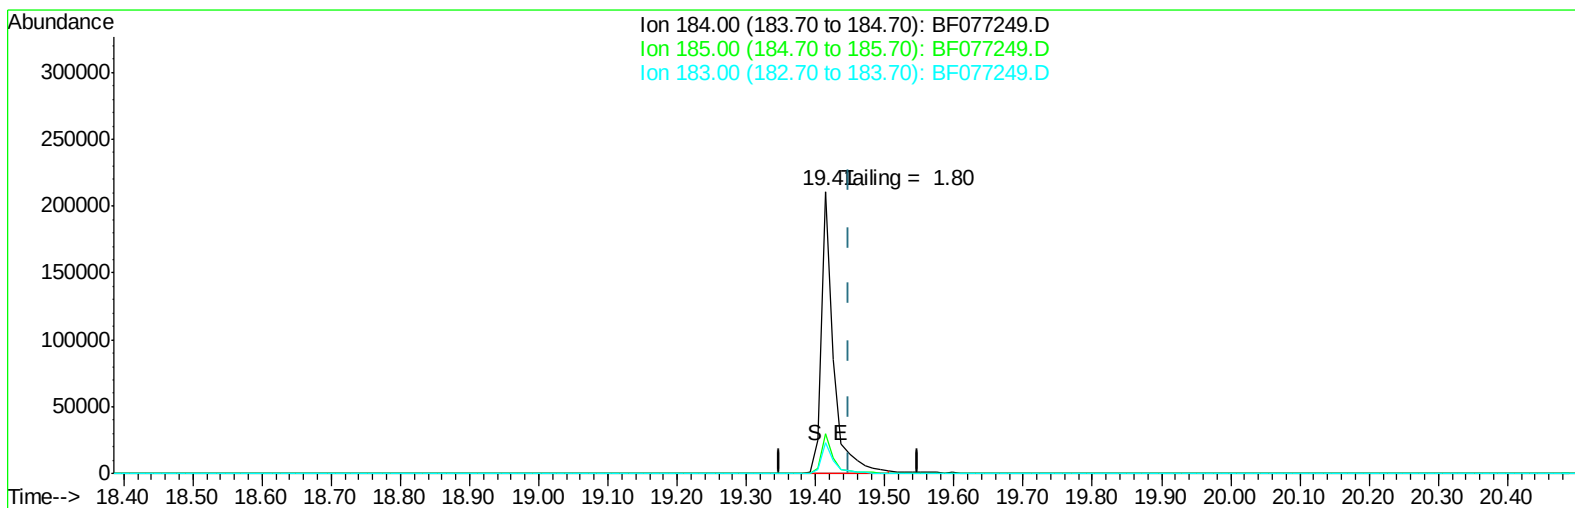

TIC: BF077249.D

(76) Benzidine

19.414min (-0.034) 0.00ng

response 262120

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.99
183.00	11.30	11.03
0.00	0.00	0.00