
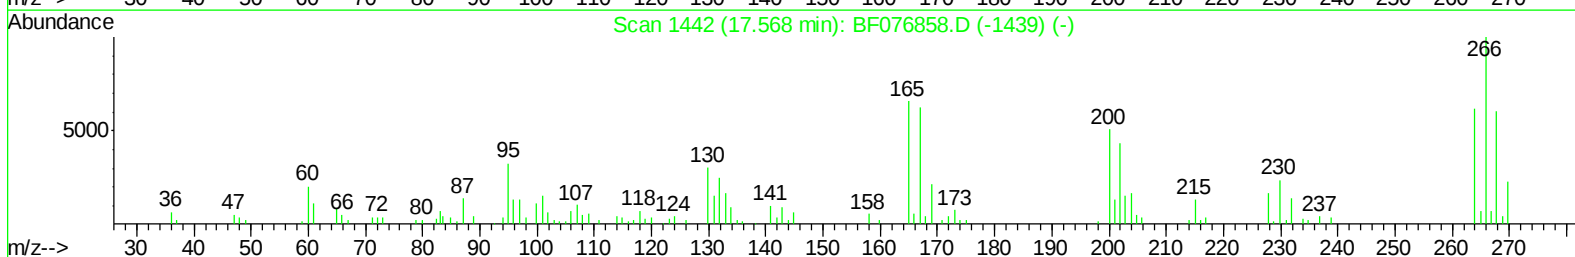
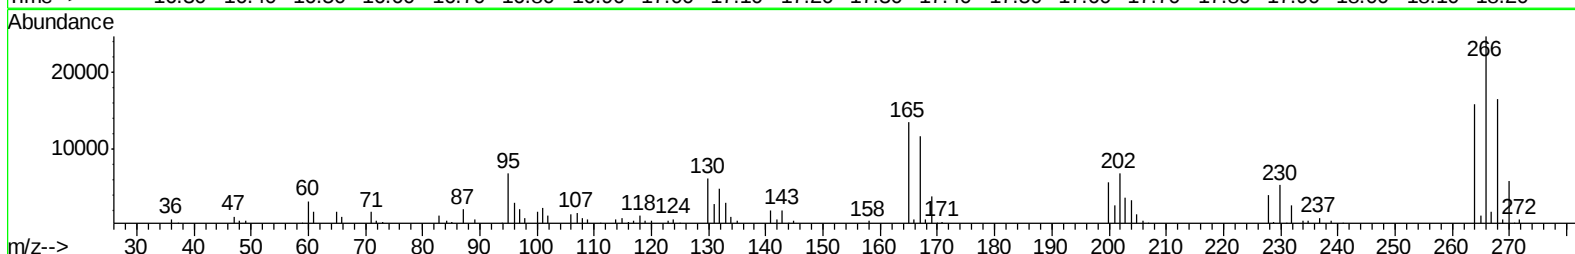


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021115\
Data File : BF077269.D
Acq On : 12 Feb 2015 2:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 03:57:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

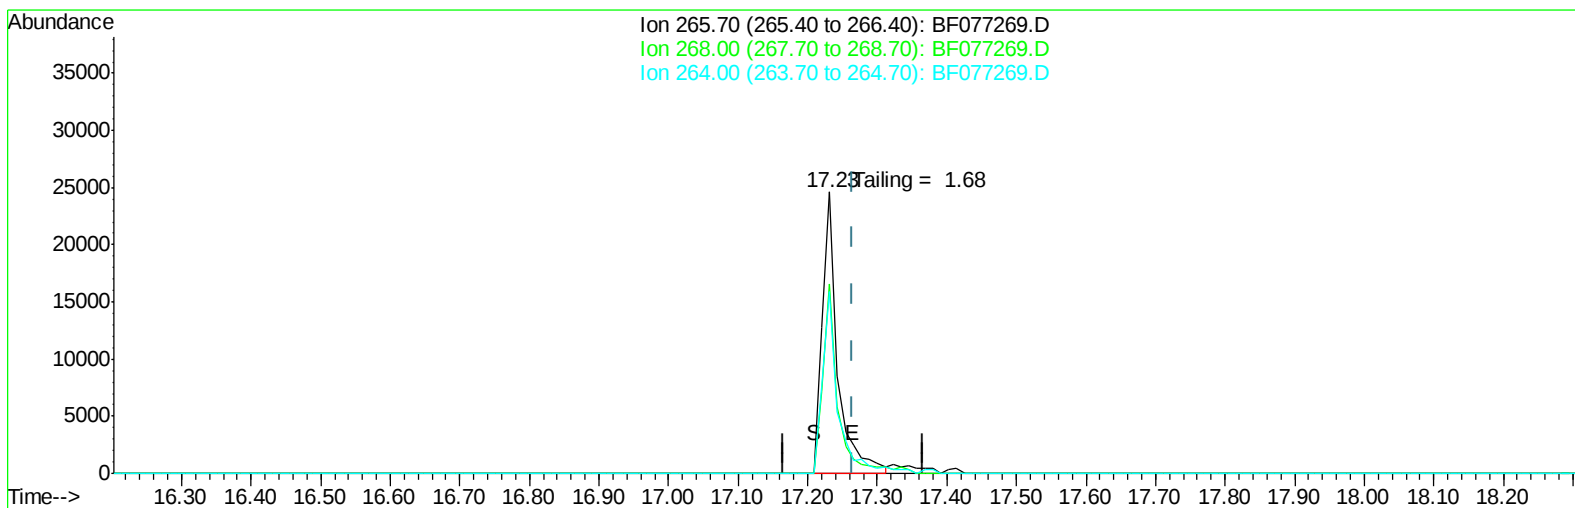

TIC: BF077269.D

(69) Pentachlorophenol (C)




17.231min (-0.034) 0.00ng

response 38511

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	67.07
264.00	61.90	64.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021115\
Data File : BF077269.D
Acq On : 12 Feb 2015 2:35
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 03:57:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

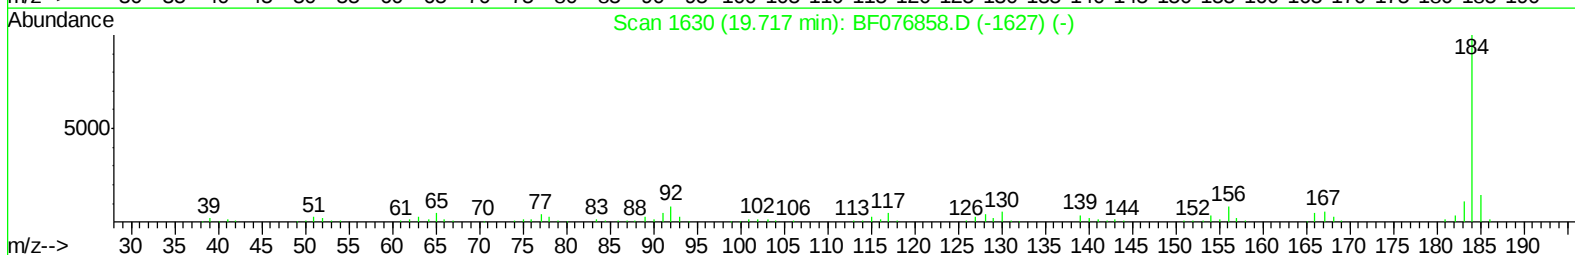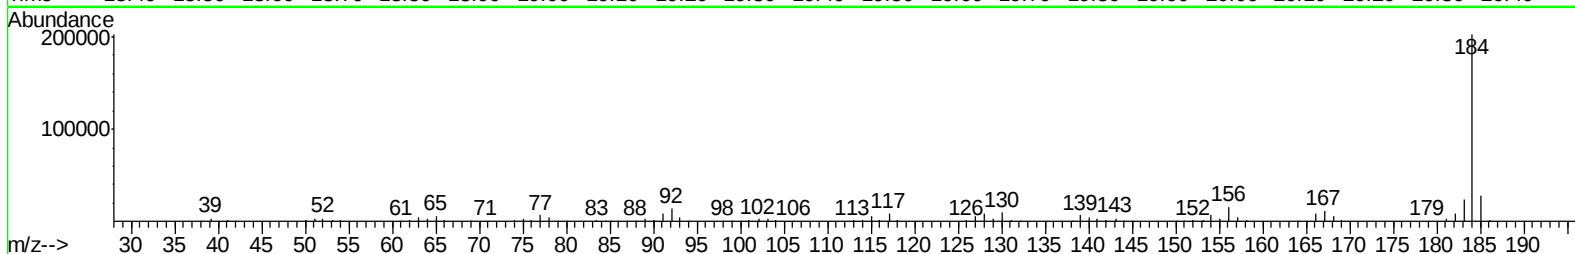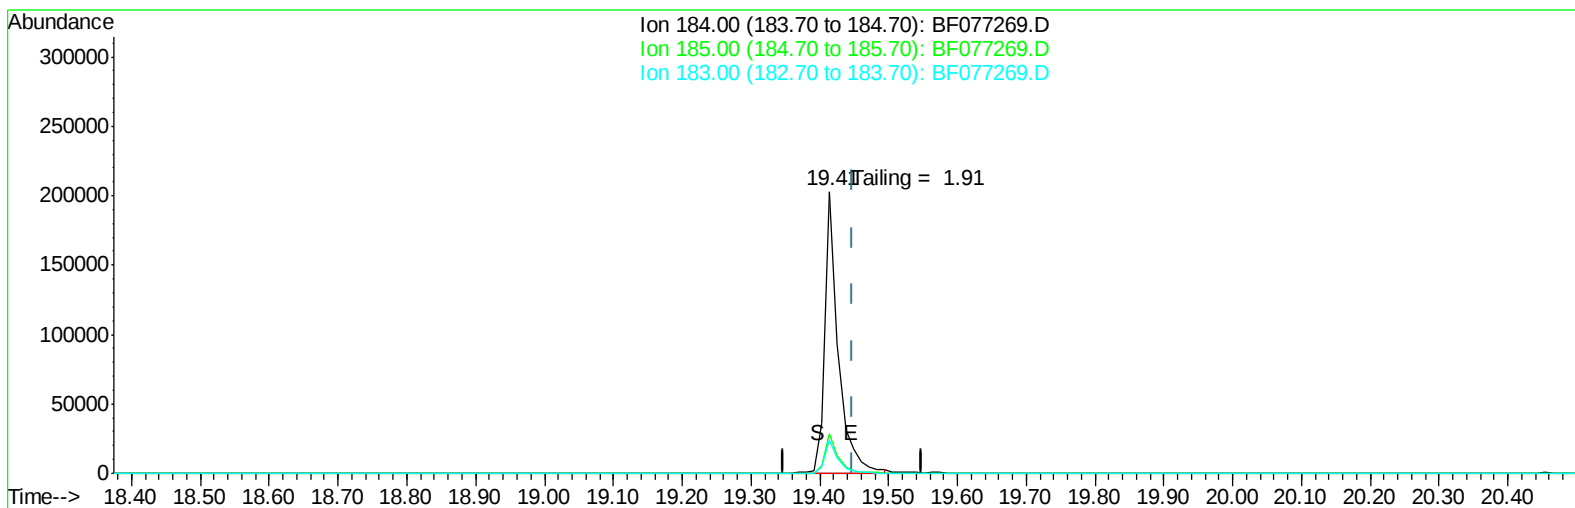

TIC: BF077269.D

(76) Benzidine

19.414min (-0.034) 0.00ng

response 271218

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.05
183.00	11.30	11.88
0.00	0.00	0.00