

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077255.D
 Acq On : 11 Feb 2015 15:49
 Operator : TP/IZ
 Sample : G1269-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 DCW-RB03-21015

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.287	33	35	39	rBV	5886	10611	1.04%	0.129%
2	1.344	39	40	50	rVV	157461	272247	26.75%	3.318%
3	3.550	230	233	243	rBV	22368	66092	6.49%	0.806%
4	4.556	318	321	333	rBV	104890	265973	26.13%	3.242%
5	6.979	530	533	536	rBV	56583	121770	11.96%	1.484%
6	7.036	536	538	548	rVB	370447	659311	64.77%	8.036%
7	7.539	579	582	590	rVB	214479	356163	34.99%	4.341%
8	7.859	607	610	618	rVB	377324	611857	60.11%	7.458%
9	8.853	694	697	705	rBV	313322	506573	49.77%	6.174%
10	10.453	834	837	844	rBV	308265	492191	48.35%	5.999%
11	11.962	965	969	974	rVB3	7960	16041	1.58%	0.196%
12	13.105	1066	1069	1073	rBV	560957	996751	97.92%	12.149%
13	14.568	1194	1197	1203	rVB2	303886	533994	52.46%	6.509%
14	16.283	1345	1347	1349	rBV	10955	17109	1.68%	0.209%
15	16.328	1349	1351	1359	rVB	337467	561295	55.14%	6.841%
16	17.471	1448	1451	1454	rBV	422619	539651	53.02%	6.578%
17	18.843	1569	1571	1578	rBV	28009	50892	5.00%	0.620%
18	19.723	1645	1648	1651	rVB	936339	1017902	100.00%	12.407%
19	20.980	1755	1758	1761	rBV	505046	563343	55.34%	6.866%
20	22.363	1877	1879	1880	rVB	18137	20764	2.04%	0.253%
21	22.626	1899	1902	1905	rBV	412158	499887	49.11%	6.093%
22	22.878	1921	1924	1927	rBV3	4755	11861	1.17%	0.145%
23	23.586	1983	1986	1991	rBV7	4735	12005	1.18%	0.146%


Sum of corrected areas: 8204283

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077255.D
Acq On : 11 Feb 2015 15:49
Operator : TP/IZ
Sample : G1269-07
Misc :
ALS Vial : 7 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
DCW-RB03-21015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

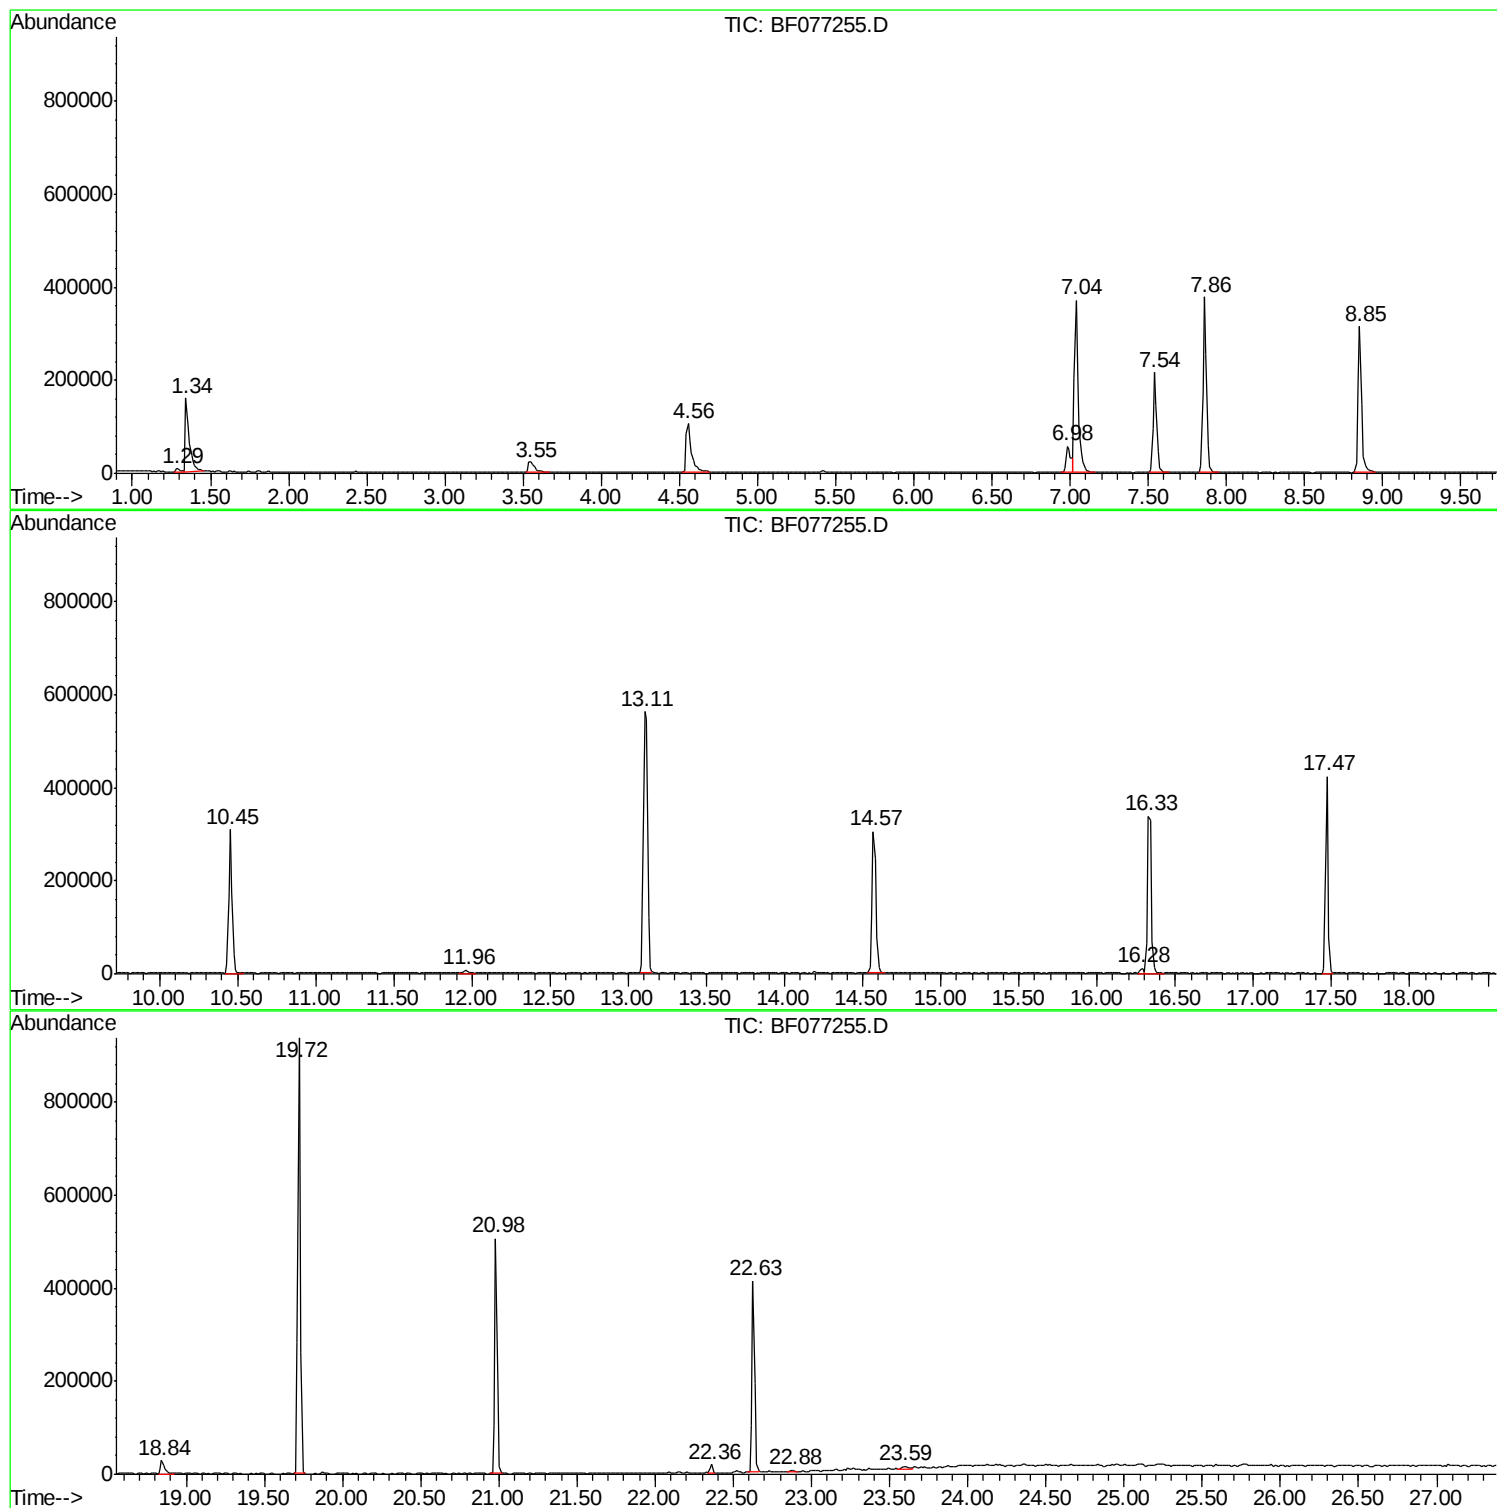

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077255.D
Acq On : 11 Feb 2015 15:49
Operator : TP/IZ
Sample : G1269-07
Misc :
ALS Vial : 7 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
DCW-RB03-21015










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.04 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	37.02 ng	659311	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	35
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	22
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

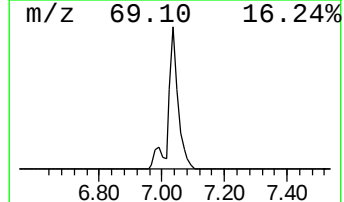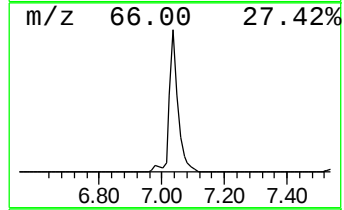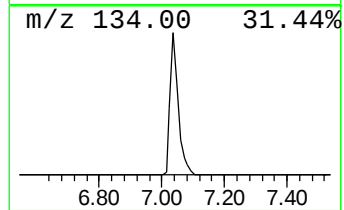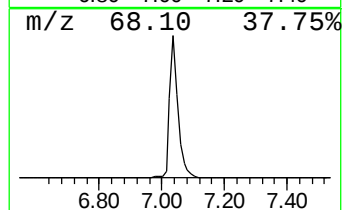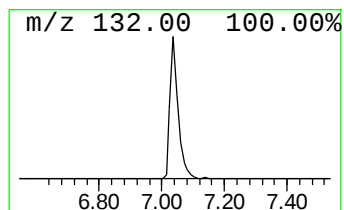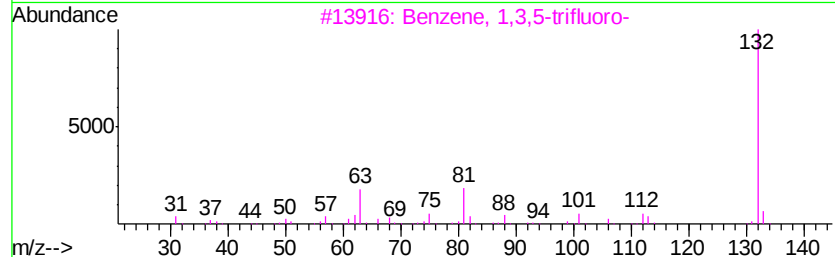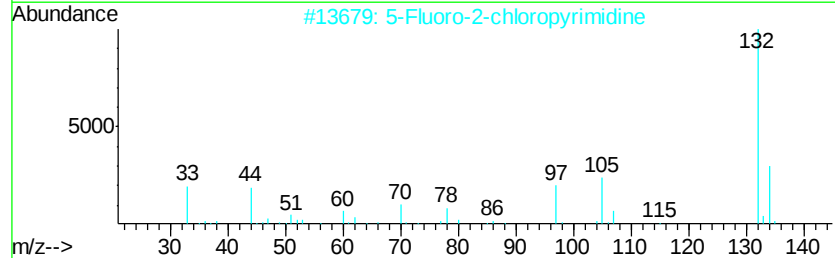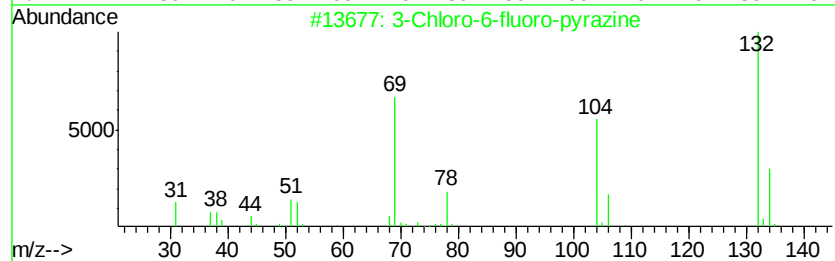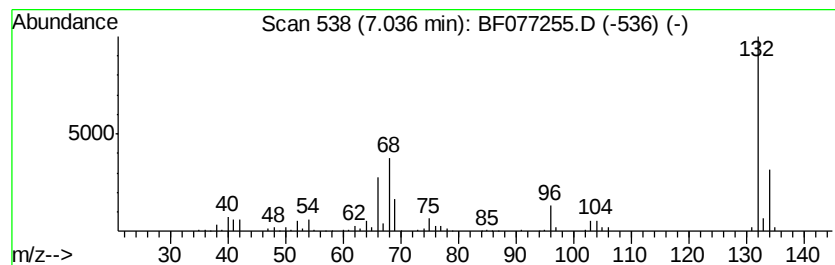

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077255.D
Acq On : 11 Feb 2015 15:49
Operator : TP/IZ
Sample : G1269-07
Misc :
ALS Vial : 7 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
DCW-RB03-21015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.04	7.04	37.0	ng	659311	1	7.54	356163	20.0