

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077256.D
 Acq On : 11 Feb 2015 16:24
 Operator : TP/IZ
 Sample : PB81702BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 PB81702BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	33	34	39	rBV	269653	453782	42.36%	4.075%
2	1.344	39	40	55	rVB	539842	978685	91.36%	8.790%
3	3.550	230	233	244	rBV	71887	212026	19.79%	1.904%
4	4.544	318	320	334	rBV	330588	756994	70.66%	6.799%
5	6.967	529	532	535	rBV	421545	690060	64.41%	6.197%
6	7.036	535	538	545	rVB	492985	875047	81.68%	7.859%
7	7.539	579	582	592	rBV	233945	399902	37.33%	3.592%
8	7.859	607	610	619	rBV	364648	609988	56.94%	5.478%
9	8.853	694	697	706	rBV	295197	475837	44.42%	4.274%
10	10.453	833	837	848	rVB	346828	548820	51.23%	4.929%
11	13.105	1066	1069	1073	rBV	553401	973220	90.85%	8.741%
12	14.568	1194	1197	1204	rVB2	350978	625401	58.38%	5.617%
13	16.328	1349	1351	1360	rVB	368791	584033	54.52%	5.245%
14	17.471	1448	1451	1454	rBV	501641	651437	60.81%	5.851%
15	19.723	1645	1648	1651	rVB	1022534	1071282	100.00%	9.621%
16	20.980	1755	1758	1761	rBV	593317	633373	59.12%	5.688%
17	22.626	1899	1902	1905	rBV	488722	582331	54.36%	5.230%
18	23.575	1982	1985	1989	rBV6	4626	12274	1.15%	0.110%




Sum of corrected areas: 11134492

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077256.D
Acq On : 11 Feb 2015 16:24
Operator : TP/IZ
Sample : PB81702BL
Misc :
ALS Vial : 8 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB81702BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

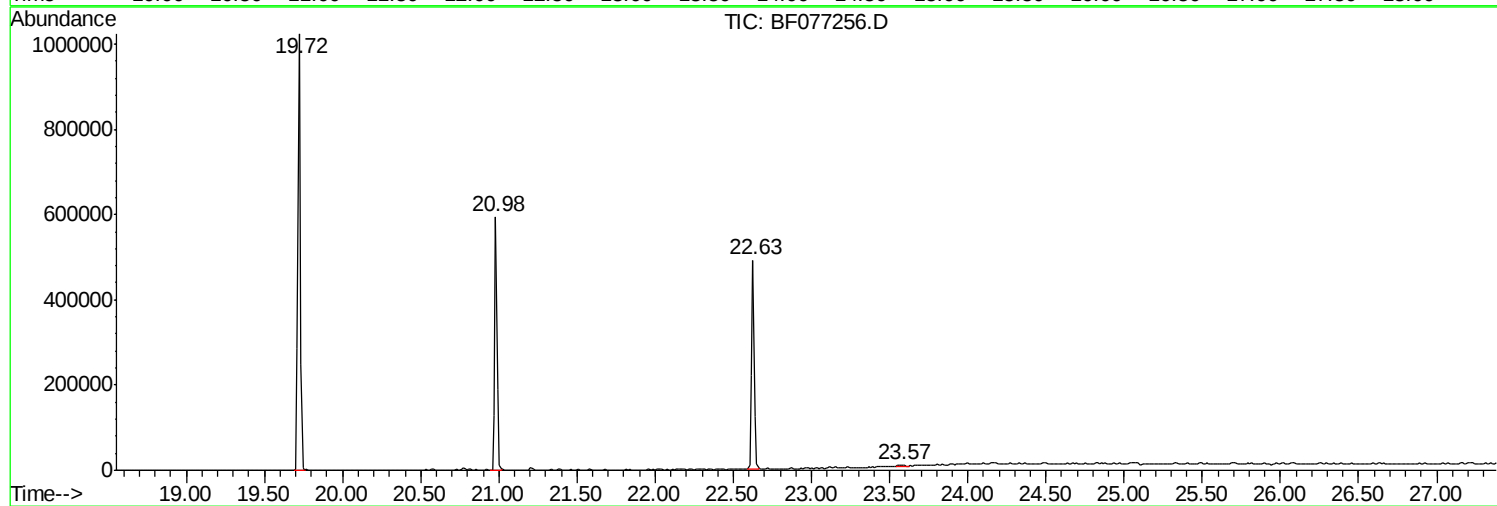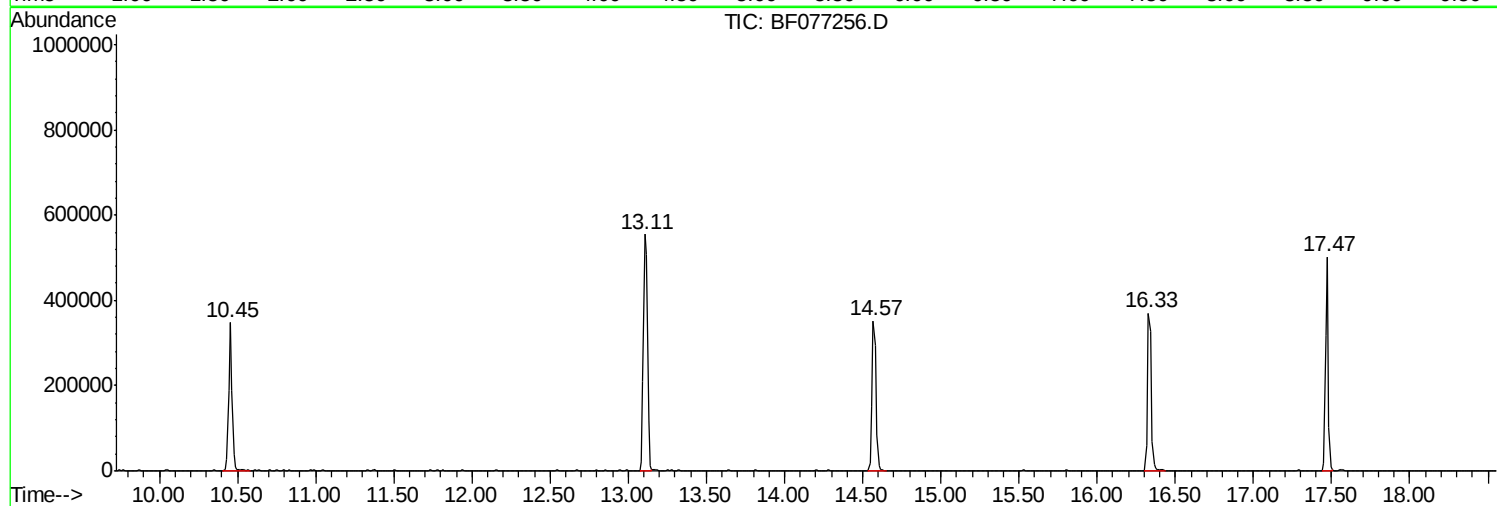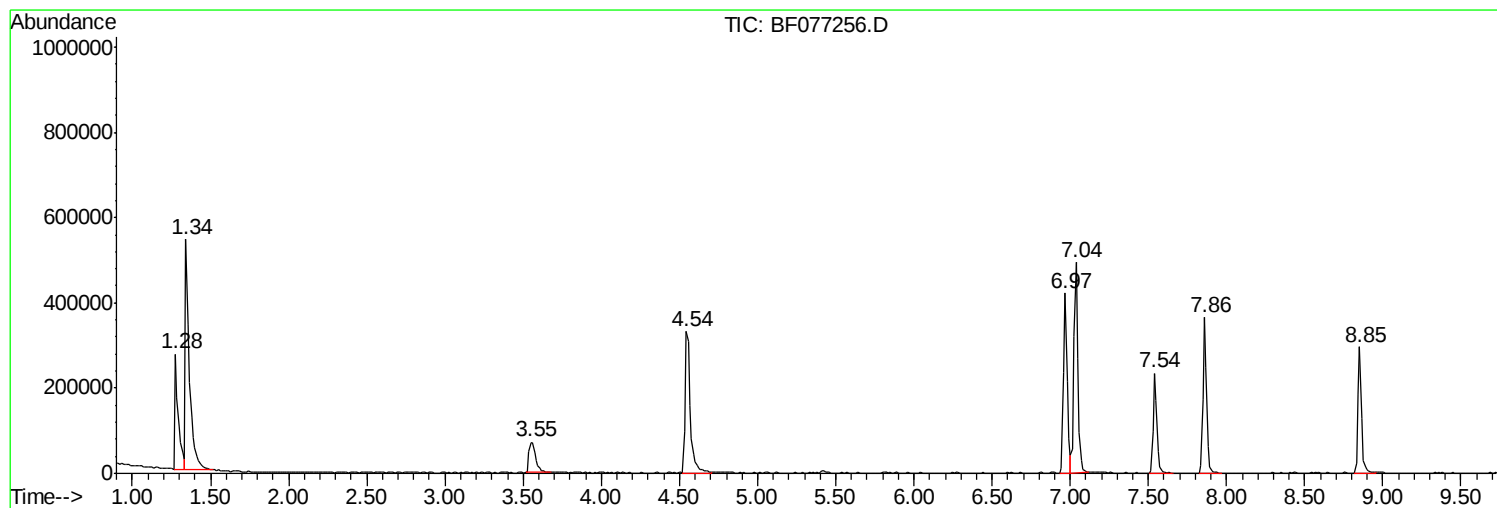

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077256.D
Acq On : 11 Feb 2015 16:24
Operator : TP/IZ
Sample : PB81702BL
Misc :
ALS Vial : 8 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampled :
PB81702BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.55	10.60 ng	212026	1,4-Dichlorobenzene-d4	7.54

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Guanidine	59	CH5N3	000113-00-8	50
3		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36
4		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
5		1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	28

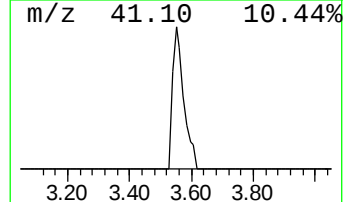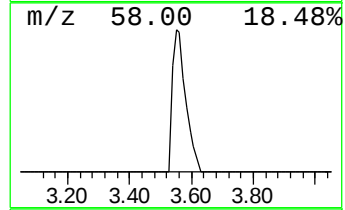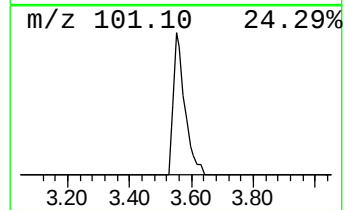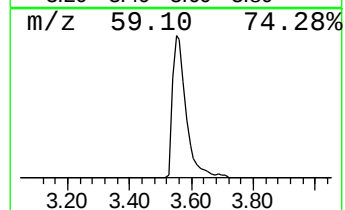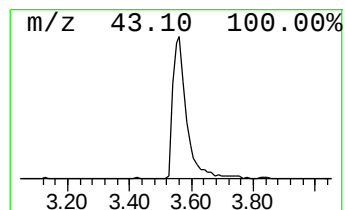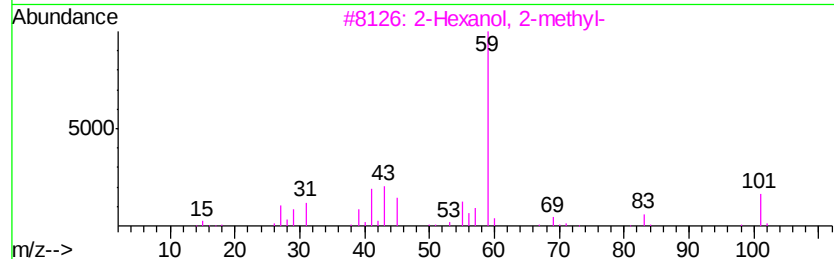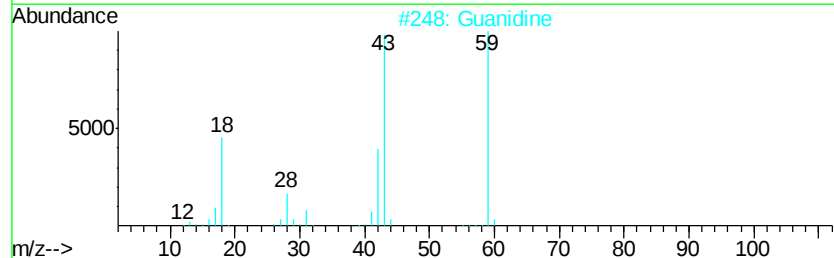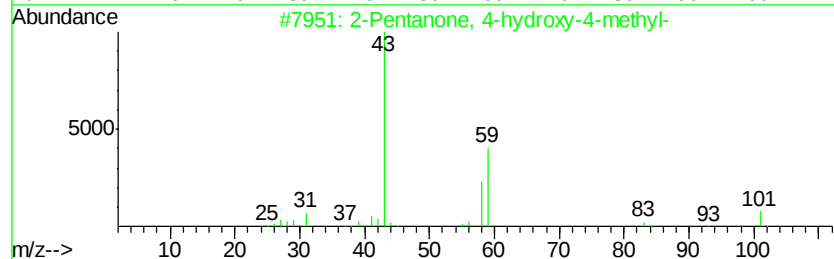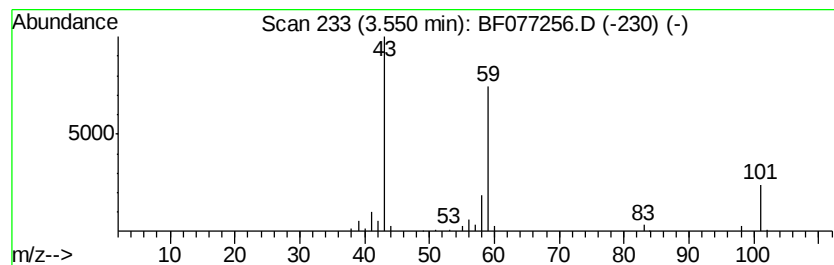

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077256.D
Acq On : 11 Feb 2015 16:24
Operator : TP/IZ
Sample : PB81702BL
Misc :
ALS Vial : 8 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB81702BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.04 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.04	43.76 ng	875047	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

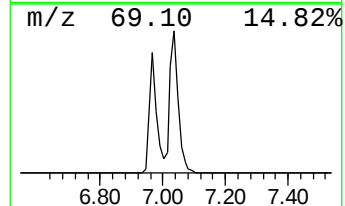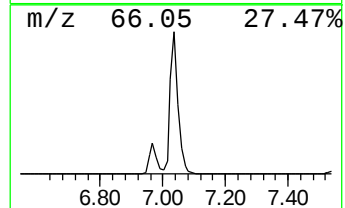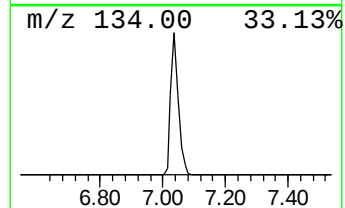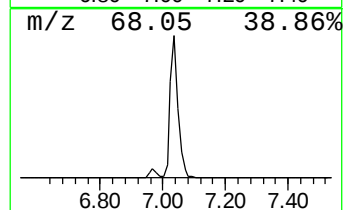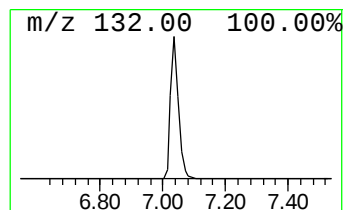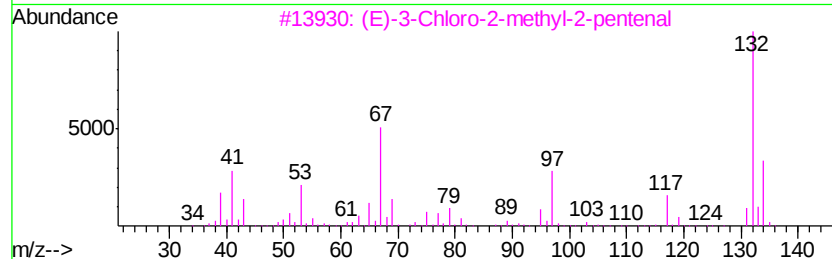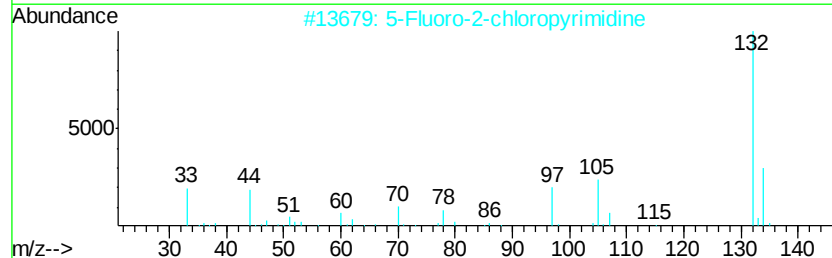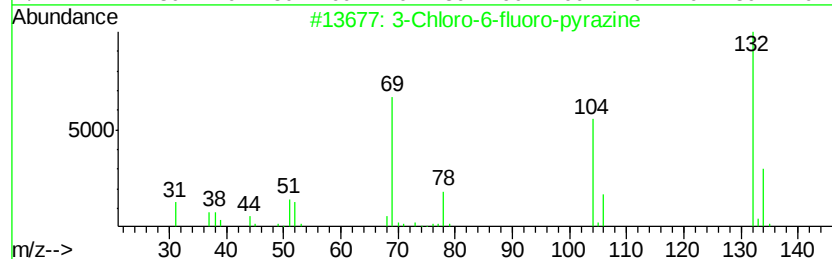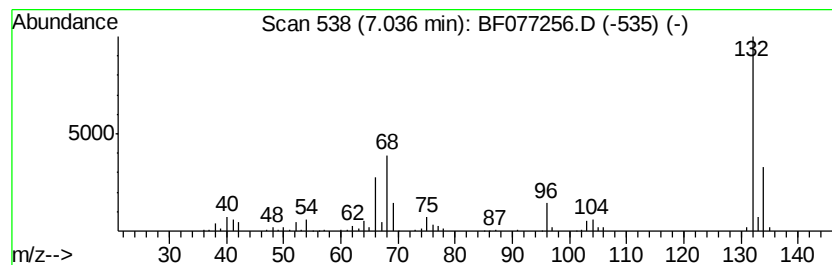

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077256.D
Acq On : 11 Feb 2015 16:24
Operator : TP/IZ
Sample : PB81702BL
Misc :
ALS Vial : 8 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB81702BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	3.55	10.6	ng	212026	1	7.54	399902	20.0
unknown7.04	7.04	43.8	ng	875047	1	7.54	399902	20.0