

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077265.D
 Acq On : 11 Feb 2015 21:36
 Operator : TP/IZ
 Sample : G1272-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.344	39	40	55	rVB	122890	228231	14.15%	0.882%
2	2.521	140	143	148	rBB	49921	103491	6.41%	0.400%
3	3.539	229	232	250	rBB	109443	298348	18.49%	1.153%
4	4.544	317	320	335	rBV	423282	916452	56.81%	3.540%
5	6.968	529	532	535	rBV	537567	900804	55.84%	3.480%
6	7.036	535	538	544	rVB	621698	1101561	68.28%	4.255%
7	7.333	560	564	569	rVB	41762	80877	5.01%	0.312%
8	7.539	579	582	588	rBV	110282	202569	12.56%	0.783%
9	7.859	607	610	614	rVV	461061	764545	47.39%	2.953%
10	8.373	649	655	659	rBV3	21625	51681	3.20%	0.200%
11	8.853	694	697	702	rBV	388736	641301	39.75%	2.477%
12	9.139	719	722	726	rVB	129254	238974	14.81%	0.923%
13	9.356	736	741	743	rBV3	20588	49572	3.07%	0.191%
14	9.608	761	763	768	rVB2	36138	67489	4.18%	0.261%
15	9.711	768	772	776	rBV4	29055	74264	4.60%	0.287%
16	9.779	776	778	786	rVB6	12156	50640	3.14%	0.196%
17	9.905	786	789	794	rBV3	21598	62926	3.90%	0.243%
18	10.008	794	798	803	rBV3	27348	89142	5.53%	0.344%
19	10.179	810	813	818	rBV	38650	64344	3.99%	0.249%
20	10.271	818	821	824	rVB2	39664	80807	5.01%	0.312%
21	10.454	832	837	842	rBV	202535	397804	24.66%	1.537%
22	10.534	842	844	848	rVB2	32685	52533	3.26%	0.203%
23	10.739	859	862	867	rVB	254908	431913	26.77%	1.669%
24	10.922	876	878	881	rVB	86375	148991	9.24%	0.576%
25	11.036	886	888	894	rBV4	31985	77142	4.78%	0.298%
26	11.334	910	914	918	rBV5	23925	67203	4.17%	0.260%
27	11.505	923	929	934	rVB5	40705	152661	9.46%	0.590%
28	11.608	934	938	940	rBV3	44836	103132	6.39%	0.398%
29	11.677	940	944	948	rVB3	52250	125946	7.81%	0.487%
30	11.791	949	954	956	rBV	100562	210197	13.03%	0.812%
31	11.848	956	959	963	rVB3	33302	71337	4.42%	0.276%
32	12.065	974	978	979	rVV3	28091	59678	3.70%	0.231%
33	12.202	987	990	994	rVB	364709	590065	36.57%	2.279%
34	12.419	1006	1009	1012	rVB	46843	87751	5.44%	0.339%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077265.D
 Acq On : 11 Feb 2015 21:36
 Operator : TP/IZ
 Sample : G1272-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.488	1012	1015	1019	rBV3	44816	91217	5.65%	0.352%
36	12.808	1040	1043	1047	rVB4	58634	150777	9.35%	0.582%
37	12.877	1047	1049	1051	rBV	34112	63702	3.95%	0.246%
38	12.922	1051	1053	1055	rVB2	35114	52341	3.24%	0.202%
39	12.991	1056	1059	1063	rBV4	42427	104026	6.45%	0.402%
40	13.071	1063	1066	1067	rVV2	64529	118431	7.34%	0.458%
41	13.117	1067	1070	1072	rVV	695418	1143986	70.91%	4.419%
42	13.162	1072	1074	1076	rVV	39473	65279	4.05%	0.252%
43	13.220	1076	1079	1083	rVB2	166287	320537	19.87%	1.238%
44	13.322	1085	1088	1092	rBV4	19425	53755	3.33%	0.208%
45	13.437	1095	1098	1101	rBV2	39795	94317	5.85%	0.364%
46	13.562	1104	1109	1112	rVB	456718	788187	48.85%	3.045%
47	13.677	1115	1119	1121	rBV4	27134	77770	4.82%	0.300%
48	13.825	1126	1132	1136	rBV6	35982	130445	8.09%	0.504%
49	13.905	1136	1139	1141	rVB	83819	128450	7.96%	0.496%
50	14.191	1160	1164	1169	rVV3	129923	311432	19.30%	1.203%
51	14.271	1169	1171	1172	rVV2	49872	82748	5.13%	0.320%
52	14.317	1172	1175	1178	rVV	159337	332838	20.63%	1.286%
53	14.385	1178	1181	1185	rVV3	122631	253406	15.71%	0.979%
54	14.454	1185	1187	1190	rVB	69120	117737	7.30%	0.455%
55	14.568	1194	1197	1201	rVB3	190852	374951	23.24%	1.448%
56	14.671	1201	1206	1210	rBV5	44586	139130	8.62%	0.537%
57	14.751	1210	1213	1216	rVV5	36370	90090	5.58%	0.348%
58	14.831	1216	1220	1223	rVV	522455	946357	58.66%	3.656%
59	14.923	1223	1228	1234	rVV2	51222	172074	10.67%	0.665%
60	15.243	1254	1256	1263	rVB5	38091	97325	6.03%	0.376%
61	15.403	1264	1270	1272	rBV3	68678	232216	14.39%	0.897%
62	15.471	1272	1276	1279	rVV3	78024	241178	14.95%	0.932%
63	15.528	1279	1281	1284	rVV3	49208	110969	6.88%	0.429%
64	15.585	1284	1286	1289	rVV	92711	167836	10.40%	0.648%
65	15.666	1289	1293	1296	rVB3	49204	118940	7.37%	0.459%
66	15.871	1306	1311	1315	rBV6	41849	152394	9.45%	0.589%
67	15.986	1315	1321	1324	rVV	549040	989186	61.31%	3.821%
68	16.031	1324	1325	1331	rVB3	28771	61167	3.79%	0.236%
69	16.283	1345	1347	1349	rBV	138350	187930	11.65%	0.726%
70	16.340	1349	1352	1354	rVV	485119	665675	41.26%	2.572%
71	16.397	1354	1357	1362	rVB	212260	453944	28.14%	1.754%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077265.D
 Acq On : 11 Feb 2015 21:36
 Operator : TP/IZ
 Sample : G1272-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	16.500	1363	1366	1368	rVB2	49116	81747	5.07%	0.316%
73	16.546	1368	1370	1372	rVB2	45358	59386	3.68%	0.229%
74	16.603	1372	1375	1379	rVB4	44713	108398	6.72%	0.419%
75	16.671	1379	1381	1383	rBV2	27158	51734	3.21%	0.200%
76	16.854	1394	1397	1402	rBV2	647756	1613324	100.00%	6.232%
77	17.083	1415	1417	1419	rVB2	30804	52100	3.23%	0.201%
78	17.117	1419	1420	1422	rBV2	30568	55137	3.42%	0.213%
79	17.163	1422	1424	1426	rVV2	50043	82666	5.12%	0.319%
80	17.209	1426	1428	1431	rVB2	49095	72244	4.48%	0.279%
81	17.311	1434	1437	1439	rVV2	68224	103325	6.40%	0.399%
82	17.471	1448	1451	1453	rBV	232082	272082	16.86%	1.051%
83	17.551	1456	1458	1460	rVV	530537	662577	41.07%	2.560%
84	17.586	1460	1461	1467	rVB	234479	344140	21.33%	1.329%
85	17.814	1478	1481	1484	rBV3	51032	108856	6.75%	0.421%
86	17.906	1487	1489	1491	rBV2	41154	51943	3.22%	0.201%
87	18.100	1504	1506	1509	rVB2	82115	135332	8.39%	0.523%
88	18.169	1509	1512	1514	rBV	457887	547408	33.93%	2.115%
89	18.397	1530	1532	1535	rVB3	34907	75319	4.67%	0.291%
90	18.580	1544	1548	1549	rBV4	29028	67503	4.18%	0.261%
91	18.717	1558	1560	1563	rVB	327768	356067	22.07%	1.376%
92	18.992	1581	1584	1586	rBV2	28575	48384	3.00%	0.187%
93	19.083	1591	1592	1595	rVB2	40087	57588	3.57%	0.222%
94	19.232	1603	1605	1609	rVB	227570	258284	16.01%	0.998%
95	19.632	1638	1640	1644	rBV	68127	95535	5.92%	0.369%
96	19.723	1644	1648	1651	rVB	895785	1238963	76.80%	4.786%
97	20.157	1683	1686	1689	rVB	81122	93583	5.80%	0.362%
98	20.980	1755	1758	1764	rBV	388938	509702	31.59%	1.969%
99	22.638	1901	1903	1907	rVB	210881	250501	15.53%	0.968%
100	23.278	1952	1959	1967	rBV3	34026	105235	6.52%	0.407%


Sum of corrected areas: 25886177

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077265.D
Acq On : 11 Feb 2015 21:36
Operator : TP/IZ
Sample : G1272-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
WC-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

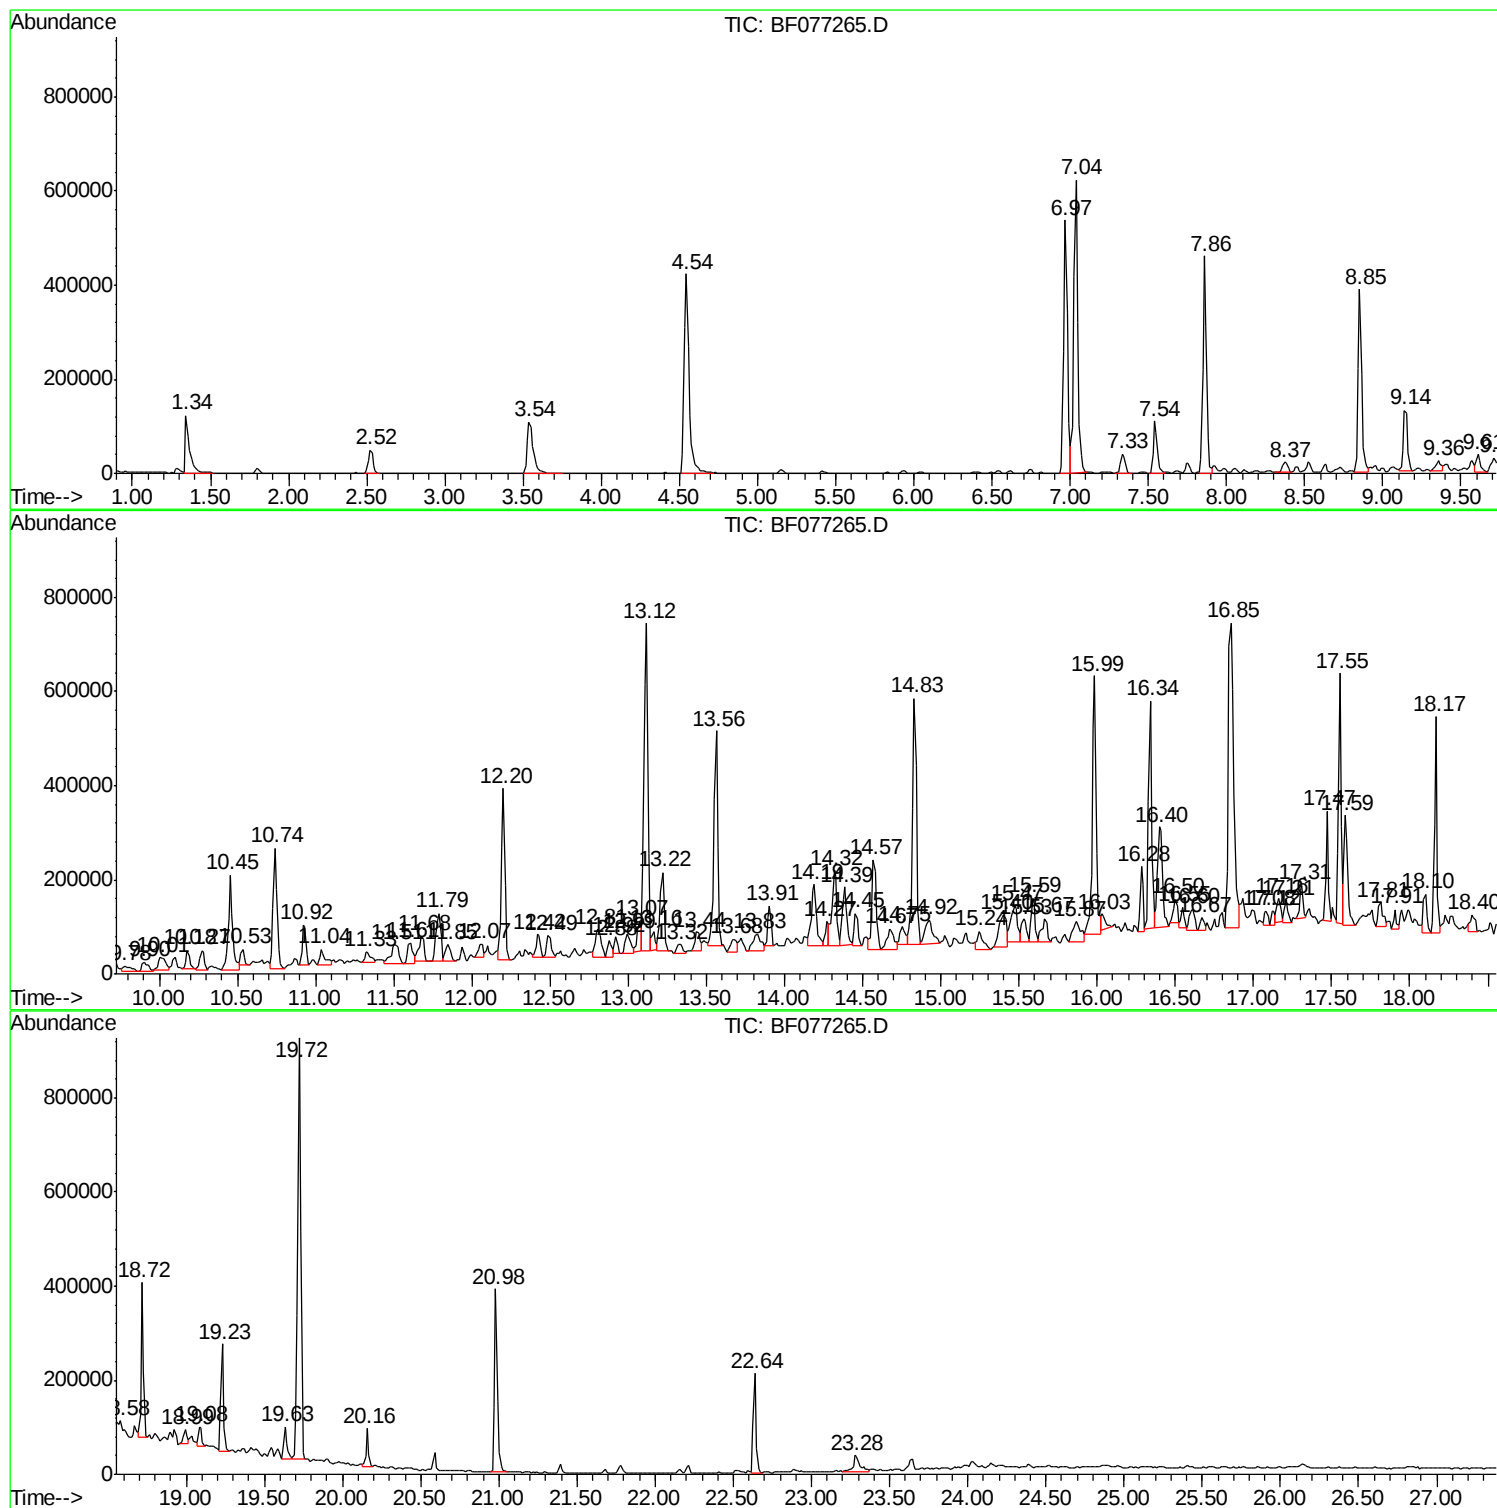

DbaaaPathh::ZZ\NRP8888M1BBAFNDATA\BBO021155\
 DbaaaFile::BB0072065DD
 Aeqq00n ::111Febb20055 221386
 Opeaaor ::TPPIZ
 Sample ::GG2222001
 Misc ::
 AASSVaal ::117 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 WC-1

QqaattMebbdd::ZZ\NRP8888M1BBAFMEH00S8200BB001445MM
 QqaattTitle ::ASBPBNASSANDABBSF00R55P000NTC6AIBBATION

TICCLibbaay ::CC\DATA\BBS6EN0\$S002LL
 TICInteggaafionPaaameess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
