

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077267.D
 Acq On : 11 Feb 2015 22:45
 Operator : TP/IZ
 Sample : PB81706TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 PB81706TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.287	32	35	39	rBV	19428	43121	3.99%	0.418%
2	1.344	39	40	52	rVB	74343	136408	12.62%	1.322%
3	3.550	230	233	245	rBV	83878	223827	20.70%	2.169%
4	4.544	317	320	337	rBV	386900	822415	76.06%	7.968%
5	6.968	529	532	535	rBV	482092	751065	69.46%	7.277%
6	7.036	535	538	546	rVB	525592	941051	87.04%	9.118%
7	7.539	579	582	591	rBB	246926	411094	38.02%	3.983%
8	7.859	607	610	618	rBV	408226	672322	62.18%	6.514%
9	8.853	694	697	713	rBB	331086	529301	48.95%	5.128%
10	10.454	834	837	847	rBV	365051	576724	53.34%	5.588%
11	13.105	1066	1069	1073	rBV	637053	1081215	100.00%	10.476%
12	14.568	1194	1197	1203	rBB2	362126	633771	58.62%	6.140%
13	16.340	1349	1352	1360	rBB	361775	593550	54.90%	5.751%
14	17.471	1448	1451	1454	rBV	495539	625234	57.83%	6.058%
15	19.632	1638	1640	1645	rBV	14504	18184	1.68%	0.176%
16	19.723	1645	1648	1651	rVV	985124	1049378	97.06%	10.167%
17	20.980	1756	1758	1761	rBV	551313	615106	56.89%	5.960%
18	22.615	1898	1901	1904	rBV	479598	583873	54.00%	5.657%
19	25.015	2103	2111	2112	rBV6	3927	13706	1.27%	0.133%


Sum of corrected areas: 10321345

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
Data File : BF077267.D
Acq On : 11 Feb 2015 22:45
Operator : TP/IZ
Sample : PB81706TB
Misc :
ALS Vial : 19 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
PB81706TB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

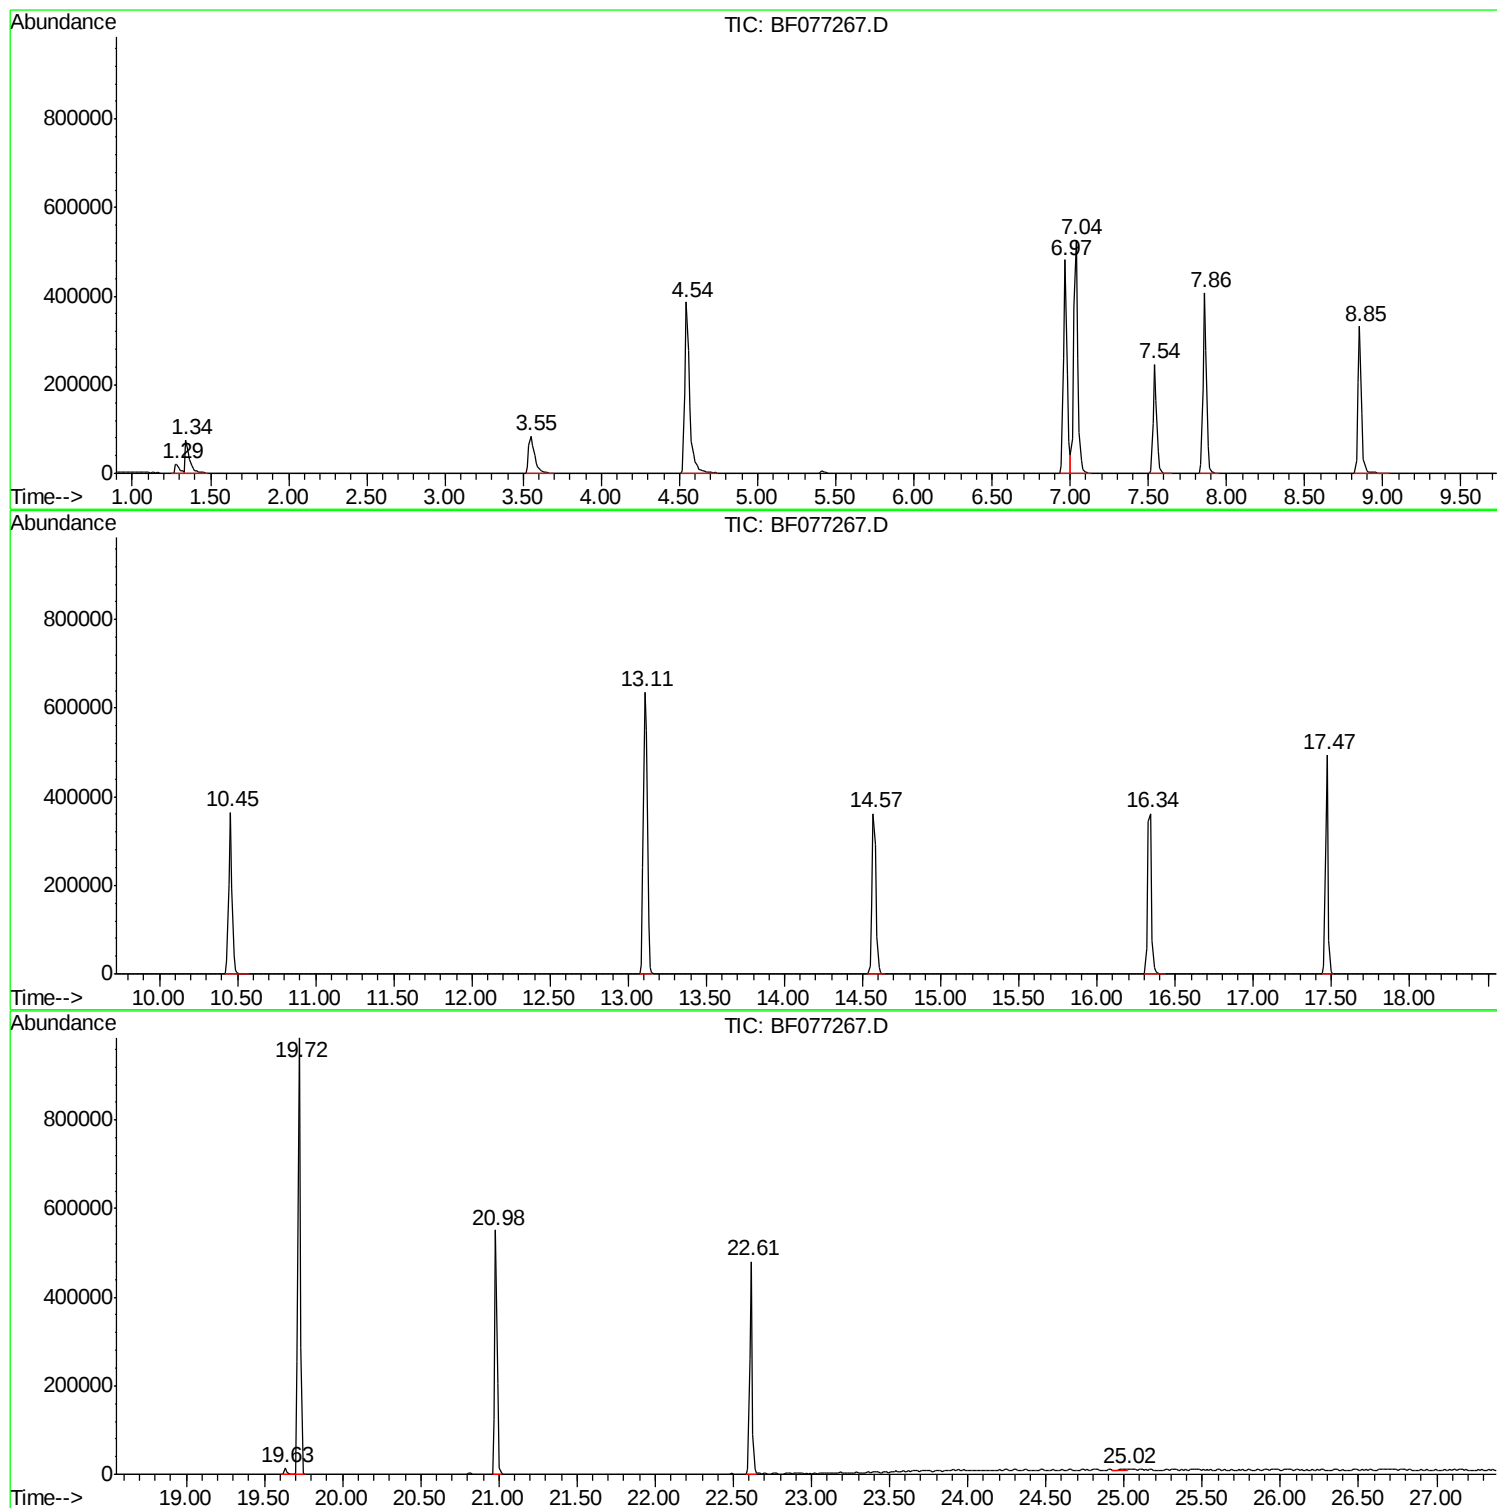

DbaaaPathh::ZZ\NRP000001\BNA\FNDA\B0021155\
 DbaaaFile::BB0072007DD
 Aeqq00n ::111Febb2005 222455
 Opeaaor ::TPPIZ
 Sample ::PB81706TB
 Misc ::
 ASSVaal ::199 SampleMultiplier:22

Instrument :
 BNA_F
 ClientSampleId :
 PB81706TB

QqaantMebbdd::ZZ\NRP000001\BNA\FNDA\B0021155\MM
 QqaantFile ::ASBPBNASSANDABBSF00R55P000NTC\BNA\B0021155\MM

TICCLibbaay ::CC\NDA\B0021155\MM
 TICCIdeggaiionPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
