


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077249.D
 Acq On : 11 Feb 2015 11:59
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 10 13:30:38 2015

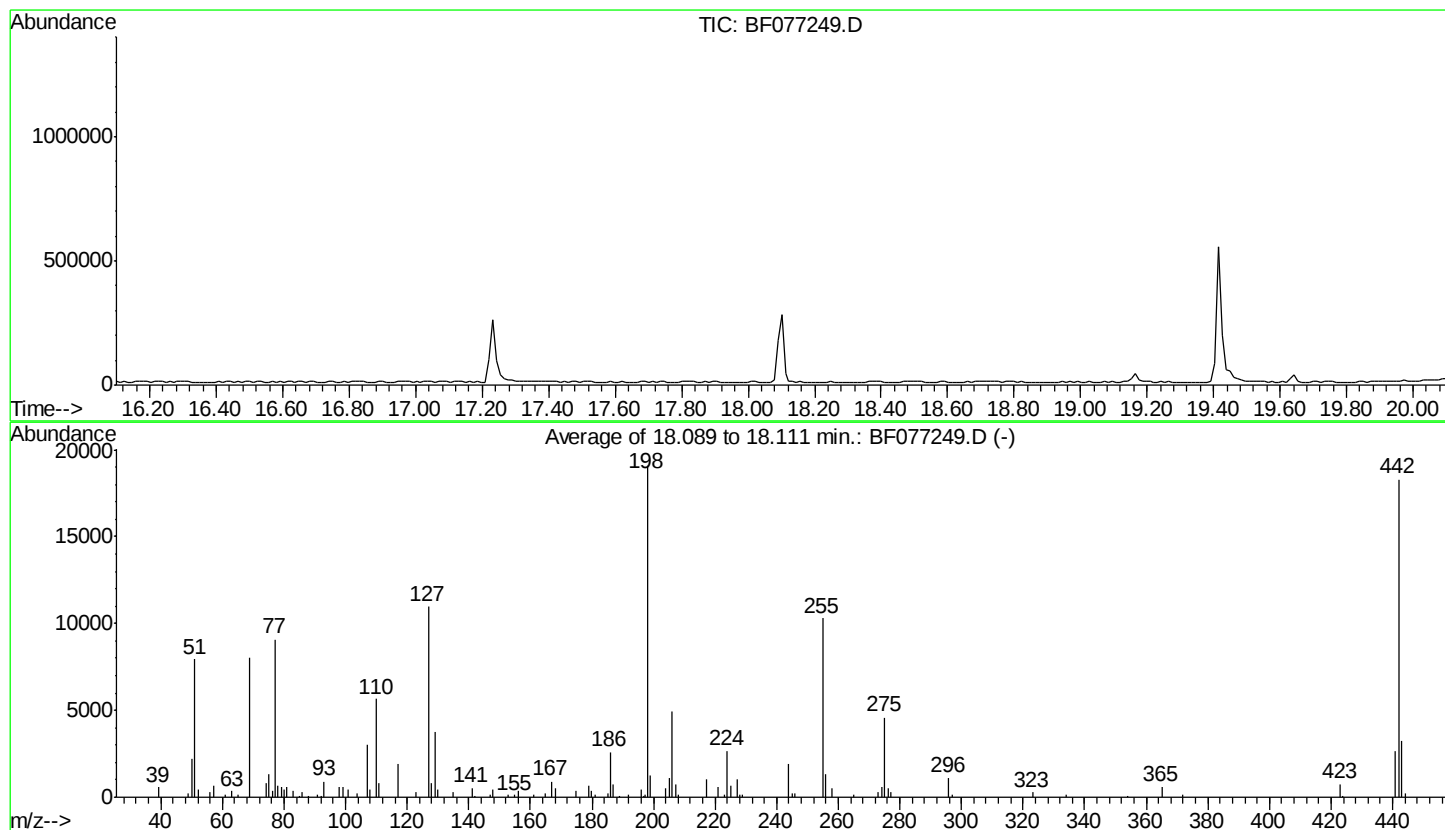

AutoFind: Scans 1505, 1506, 1507; Background Corrected with Scan 1501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	7956	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.2	8059	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.5	10970	PASS
197	198	0.00	2	0.6	119	PASS
198	198	100	100	100.0	19089	PASS
199	198	5	9	6.8	1291	PASS
275	198	10	60	24.1	4606	PASS
365	198	1	100	3.2	611	PASS
441	442	0.01	24	14.4	2632	PASS
442	198	50	100	95.8	18282	PASS
443	442	15	24	17.8	3252	PASS