


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021115\
 Data File : BF077269.D
 Acq On : 12 Feb 2015 2:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 10 13:30:38 2015

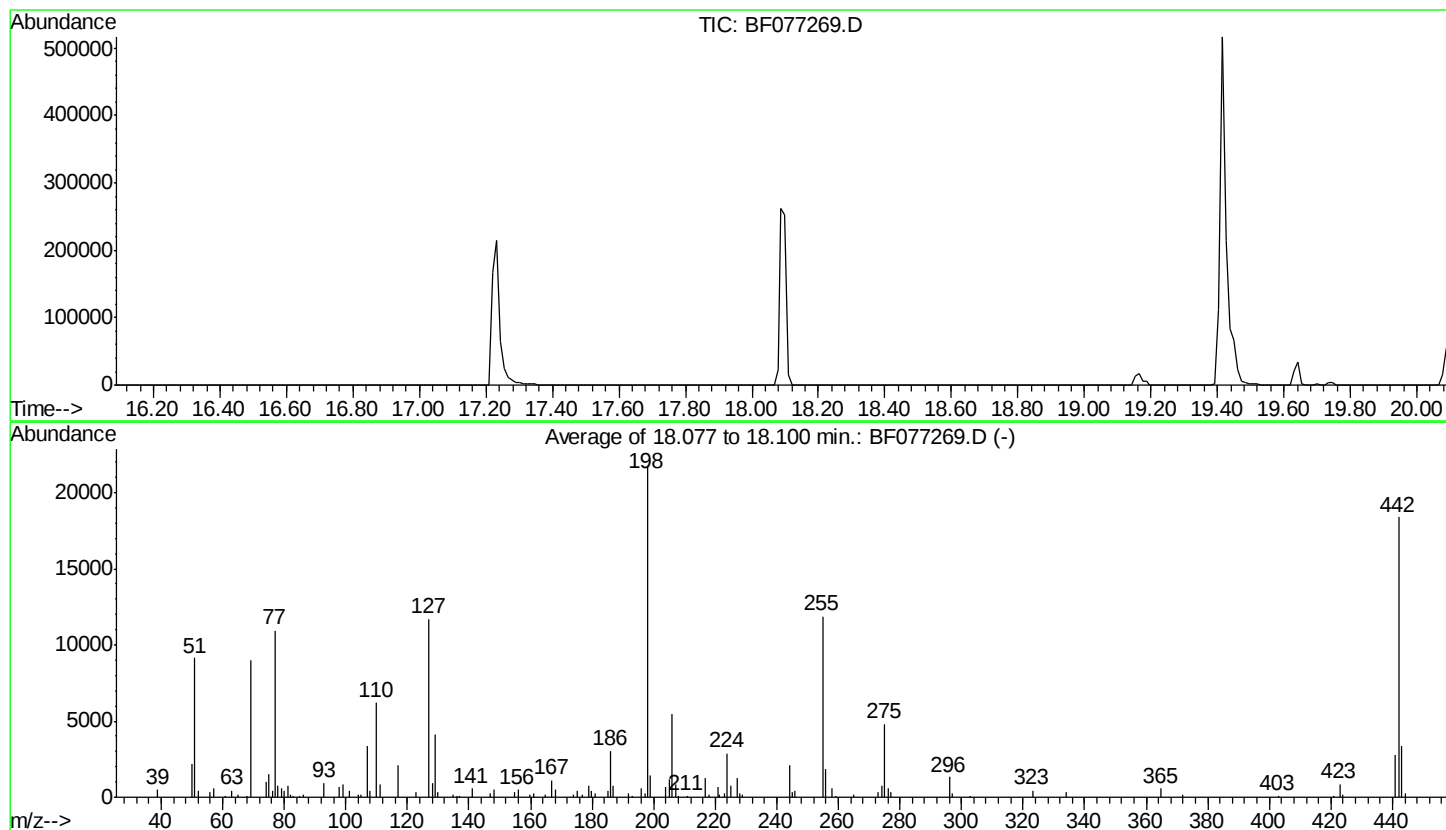

AutoFind: Scans 1504, 1505, 1506; Background Corrected with Scan 1501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	9139	PASS
68	69	0.00	2	1.4	122	PASS
69	198	0.00	100	41.3	8996	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	11682	PASS
197	198	0.00	2	1.1	234	PASS
198	198	100	100	100.0	21766	PASS
199	198	5	9	6.7	1458	PASS
275	198	10	60	22.2	4832	PASS
365	198	1	100	2.5	551	PASS
441	442	0.01	24	15.1	2776	PASS
442	198	50	100	84.5	18384	PASS
443	442	15	24	18.4	3376	PASS