
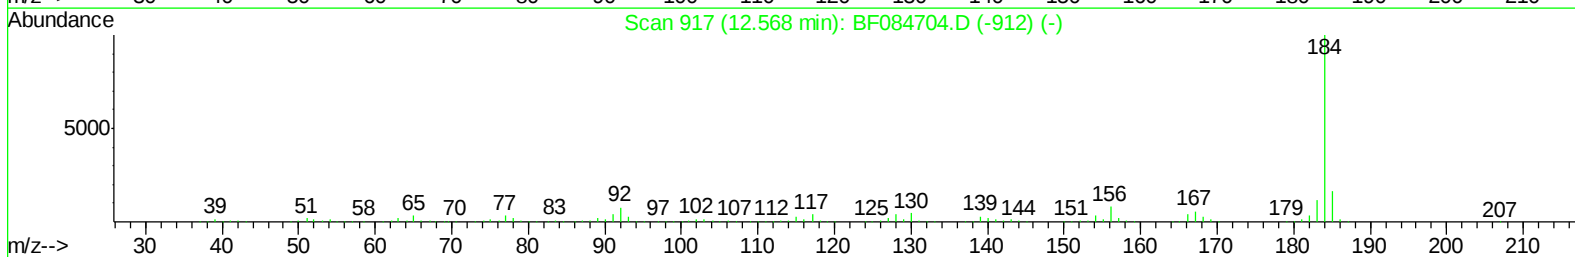
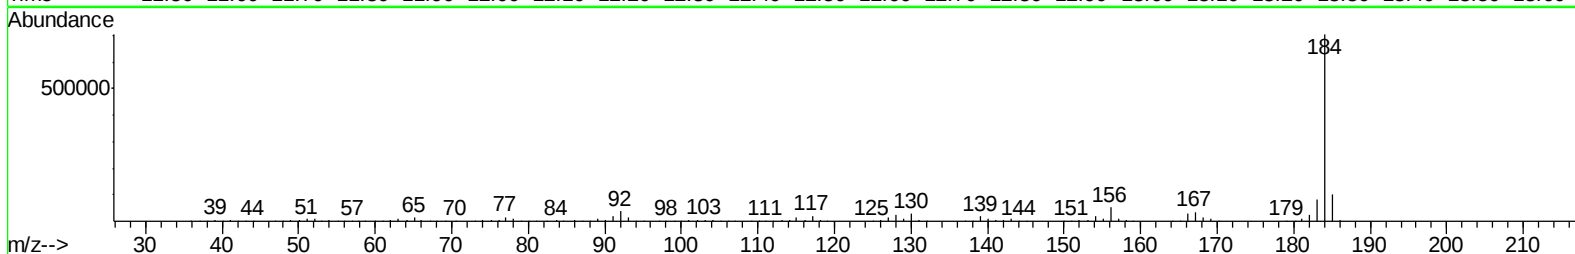


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021116\
Data File : BF085009.D
Acq On : 11 Feb 2016 10:41
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:26:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:28:51 2016
Response via : Initial Calibration

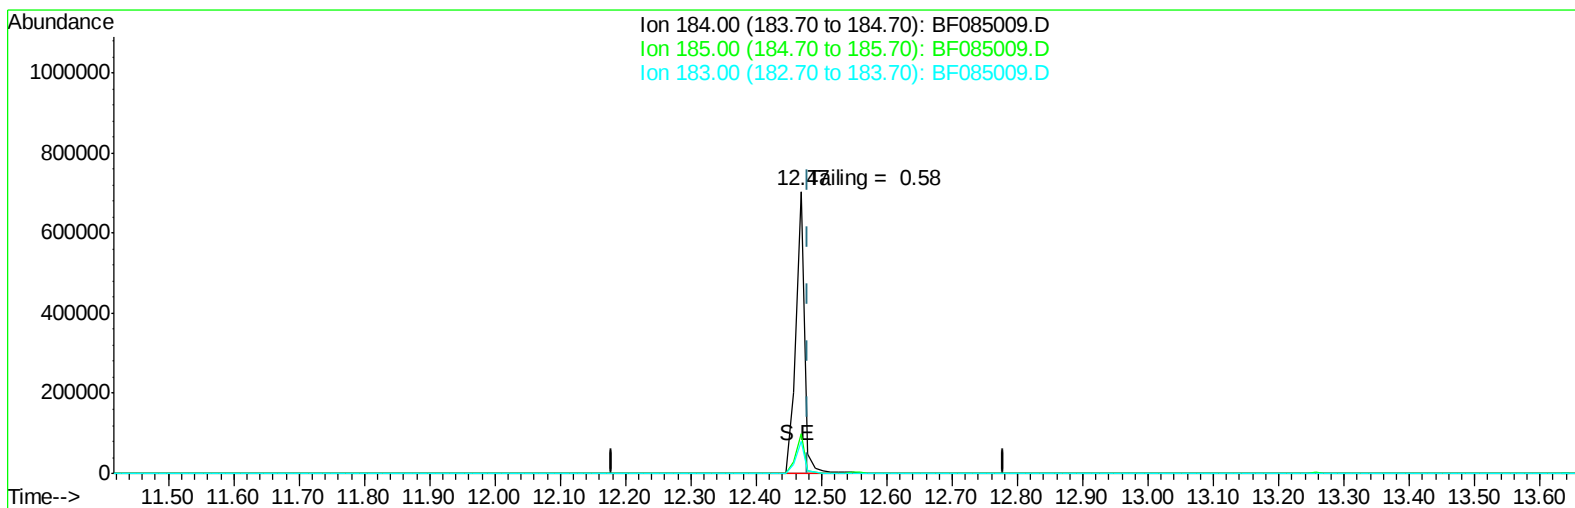

TIC: BF085009.D

(76) Benzidine




12.468min (-0.011) -20.00ng

response 683243

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.15
183.00	12.30	11.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021116\
Data File : BF085009.D
Acq On : 11 Feb 2016 10:41
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 08:26:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 13:28:51 2016
Response via : Initial Calibration

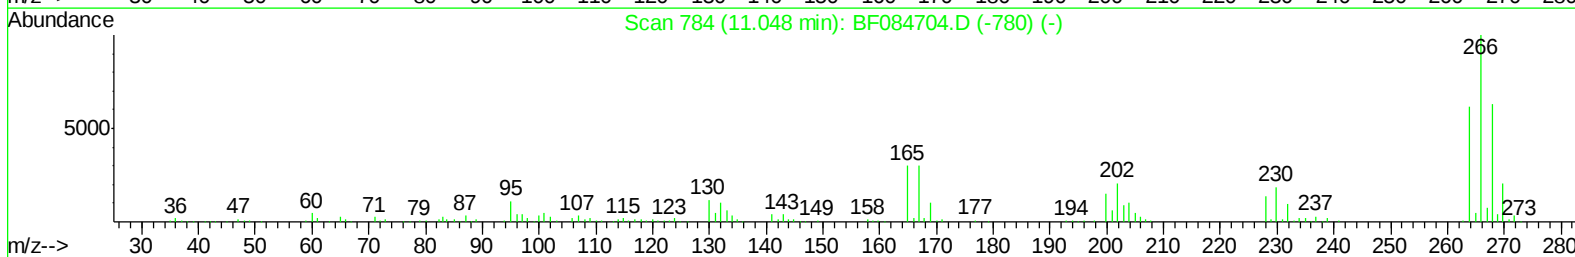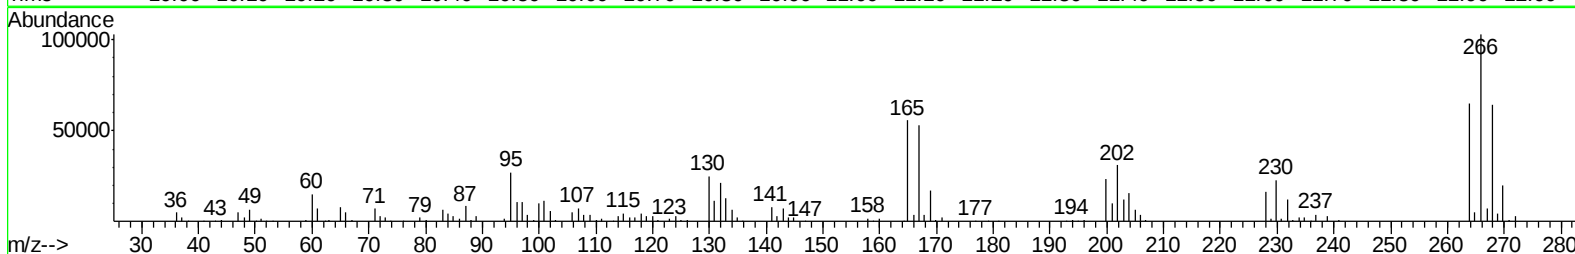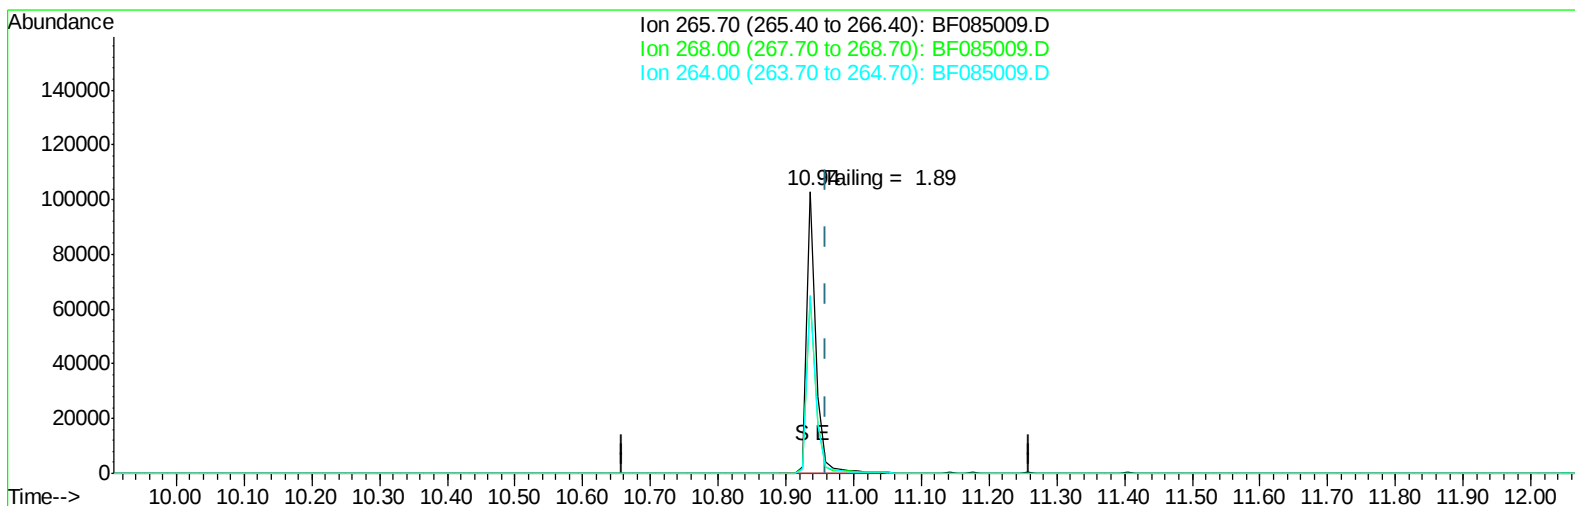

TIC: BF085009.D

(69) Pentachlorophenol (C)

10.936min (-0.023) 71697.15ng

response 98946

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	62.54
264.00	62.70	63.22
0.00	0.00	0.00