


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021116\
Data File : BF085009.D
Acq On : 11 Feb 2016 10:41
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 10 13:28:51 2016

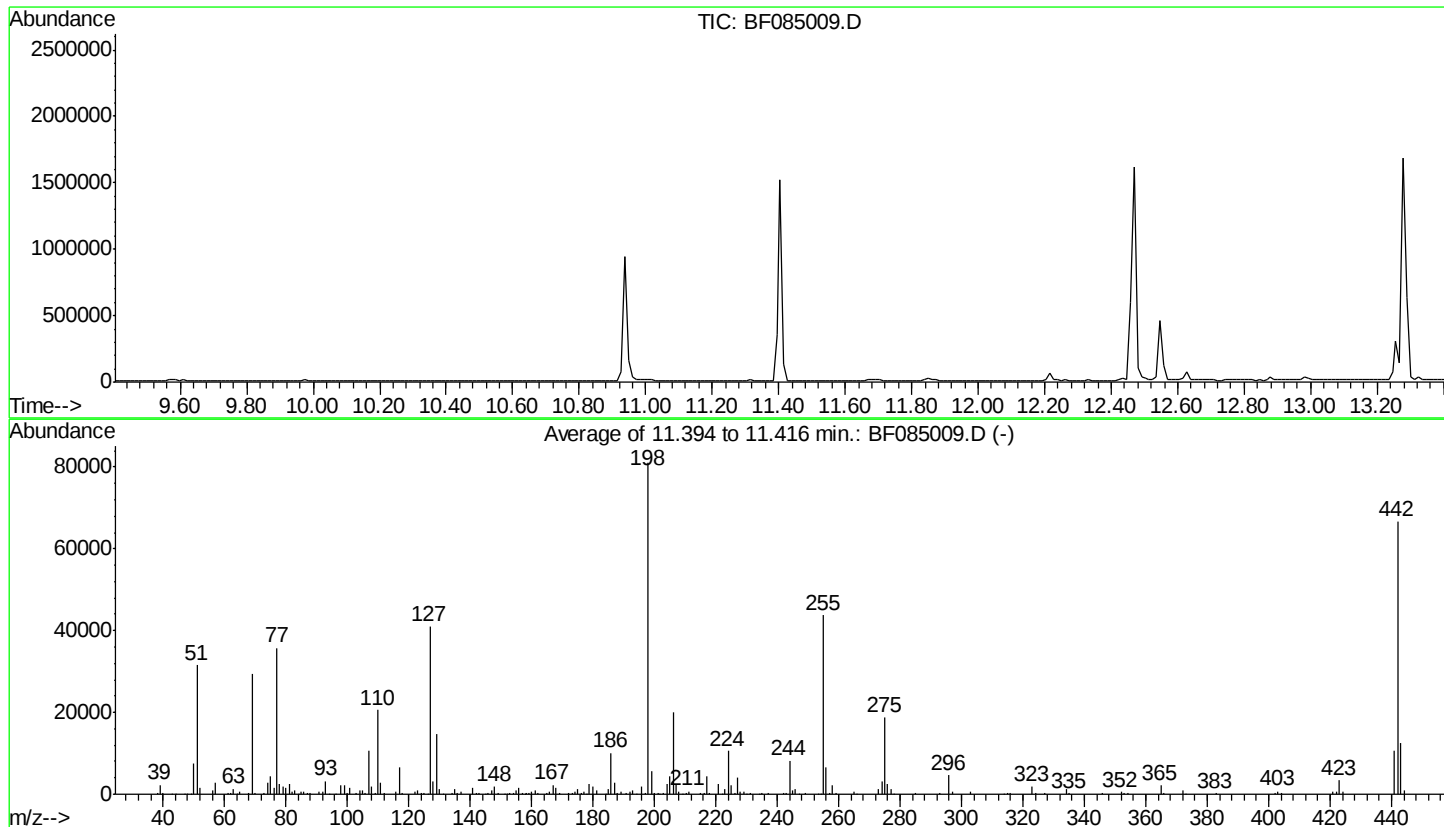

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	31593	PASS
68	69	0.00	2	1.5	441	PASS
69	198	0.00	100	36.4	29528	PASS
70	69	0.00	2	0.9	253	PASS
127	198	10	80	50.4	40883	PASS
197	198	0.00	2	0.4	355	PASS
198	198	100	100	100.0	81071	PASS
199	198	5	9	6.8	5505	PASS
275	198	10	60	23.1	18714	PASS
365	198	1	100	2.7	2153	PASS
441	442	0.01	24	15.9	10596	PASS
442	198	50	100	82.2	66632	PASS
443	442	15	24	18.9	12584	PASS