
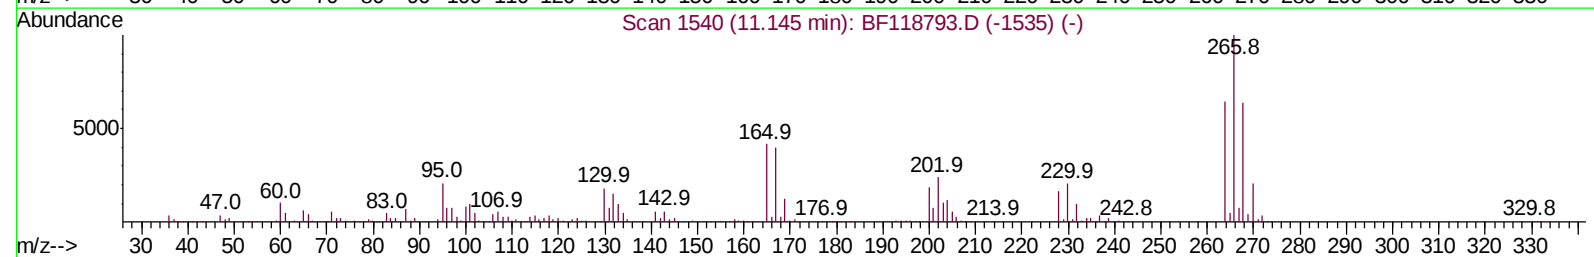
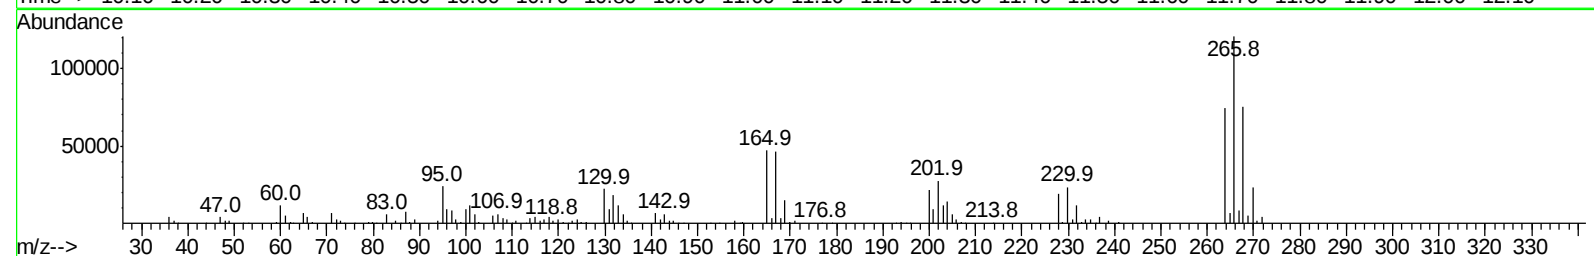


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021120\
 Data File : BF118884.D
 Acq On : 11 Feb 2020 14:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 12:04:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

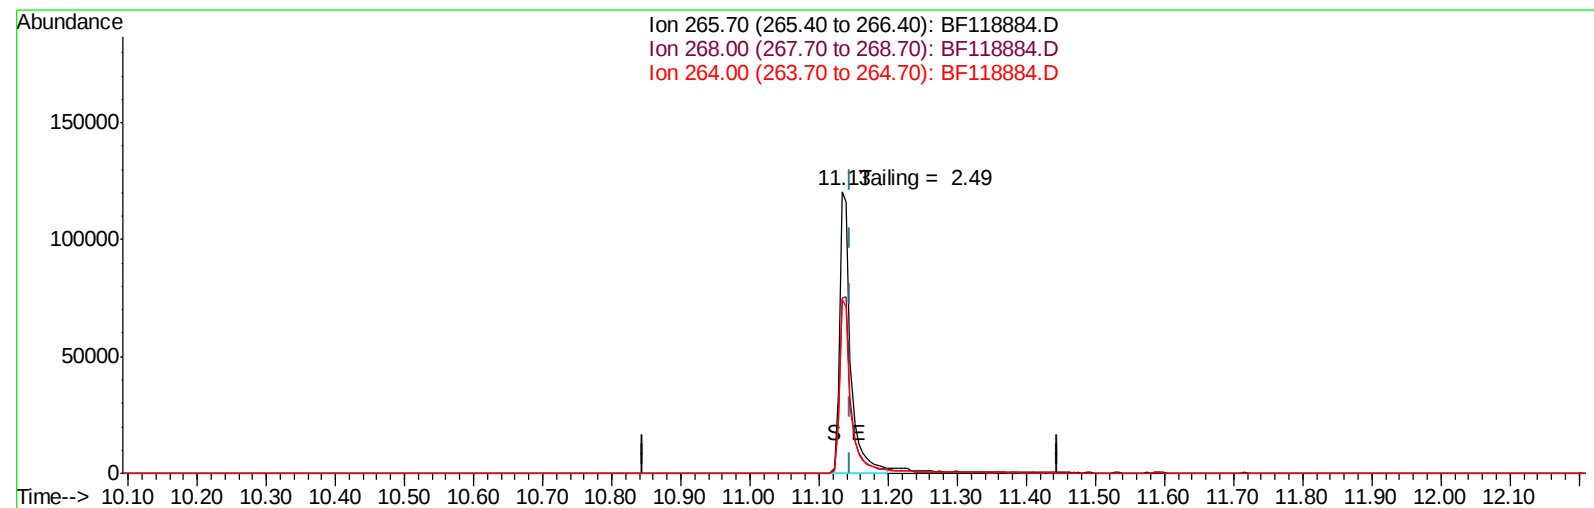

TIC: BF118884.D

(70) Pentachlorophenol (C)




11.133min (-0.012) 32595.44ng

response 138014

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.18
264.00	64.30	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF021120\
 Data File : BF118884.D
 Acq On : 11 Feb 2020 14:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 12 12:04:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF020320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 03 16:26:03 2020
 Response via : Initial Calibration

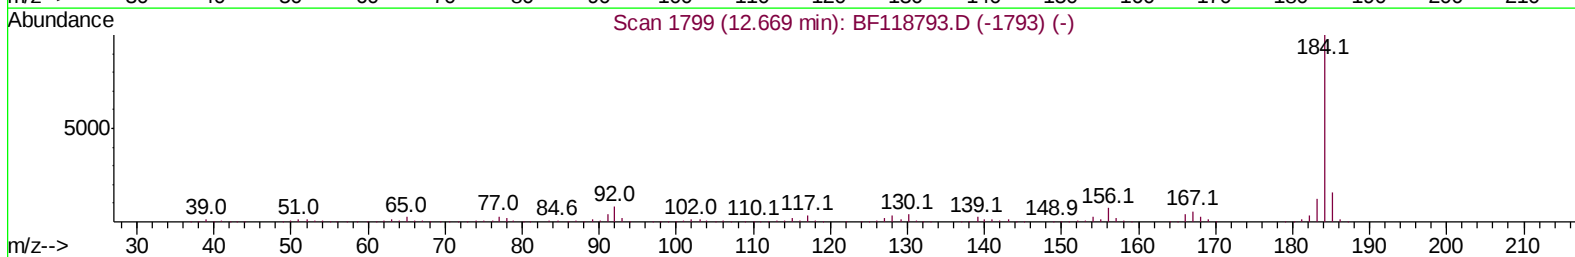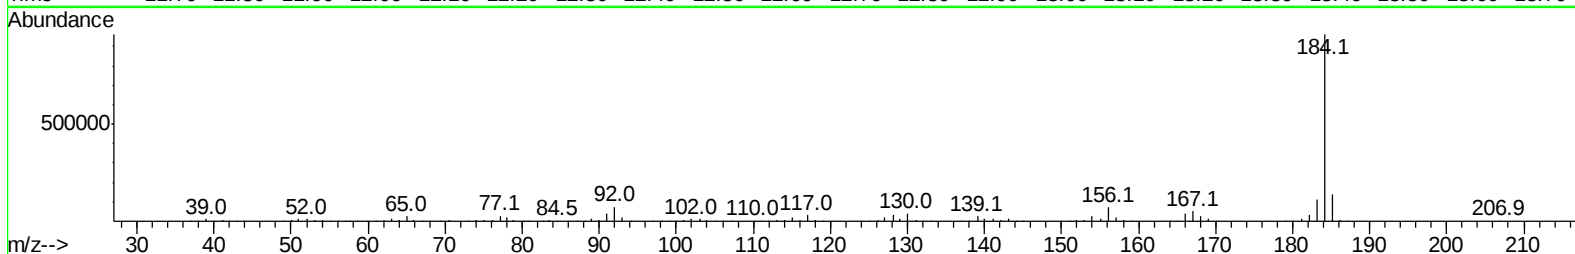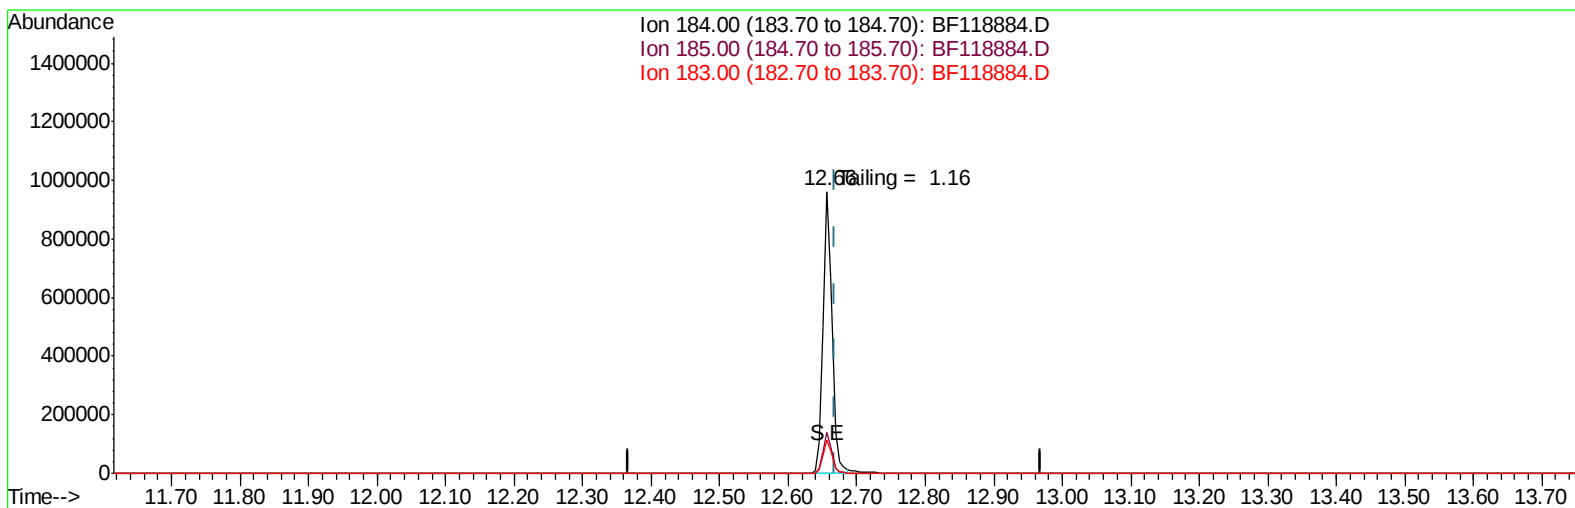

TIC: BF118884.D

(77) Benzidine

12.657min (-0.012) 0.00ng

response 881529

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.62
183.00	12.10	12.03
0.00	0.00	0.00