


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021120\
 Data File : BF118884.D
 Acq On : 11 Feb 2020 14:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF020320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 03 16:26:03 2020

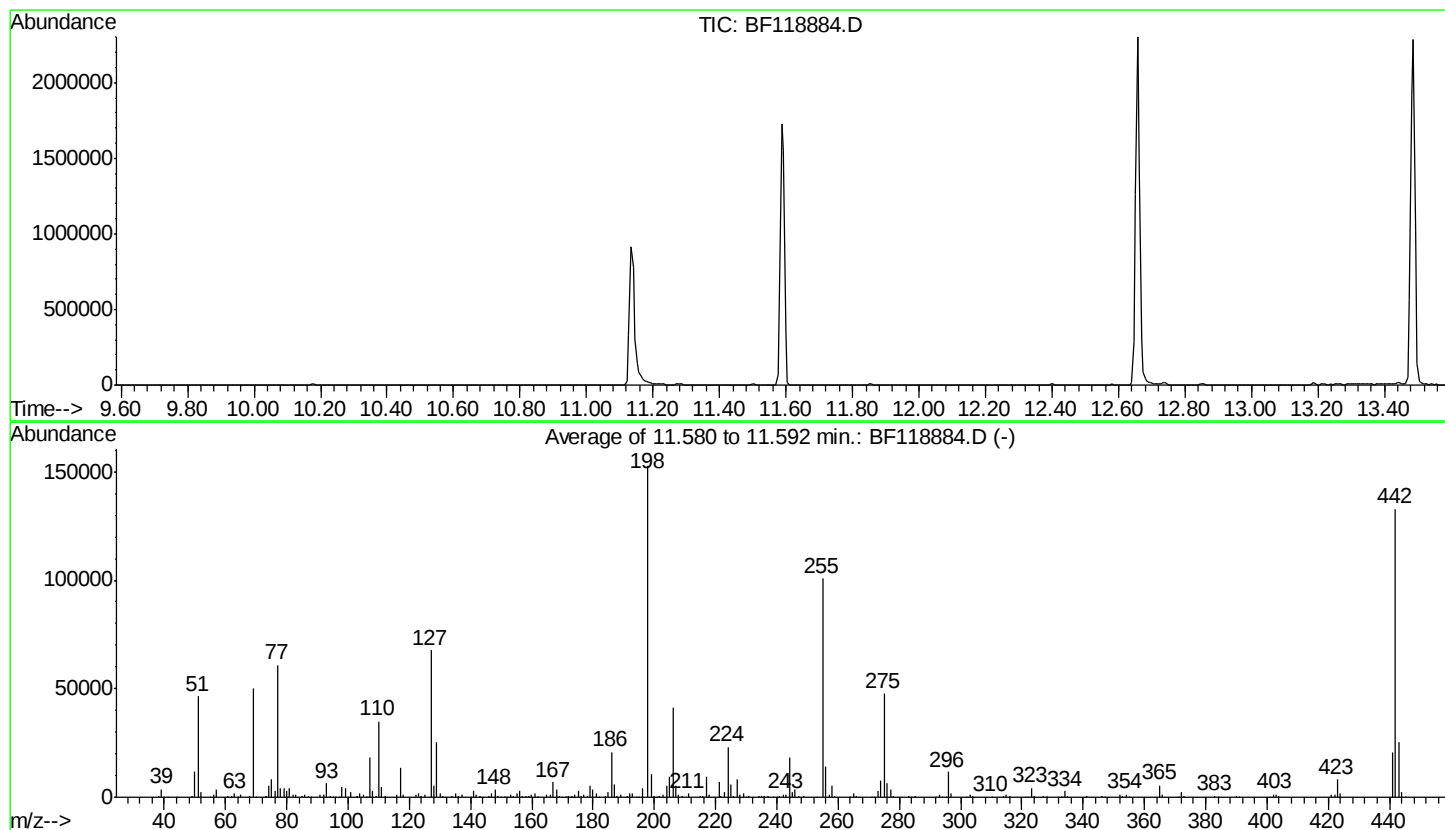

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	46336	PASS
68	69	0.00	2	1.4	678	PASS
69	198	0.00	100	32.7	50010	PASS
70	69	0.00	2	0.5	234	PASS
127	198	10	80	44.4	67813	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152810	PASS
199	198	5	9	6.9	10610	PASS
275	198	10	60	31.2	47749	PASS
365	198	1	100	3.5	5420	PASS
441	198	0.01	100	13.5	20601	PASS
442	198	50	100	86.9	132850	PASS
443	442	15	24	19.3	25615	PASS