
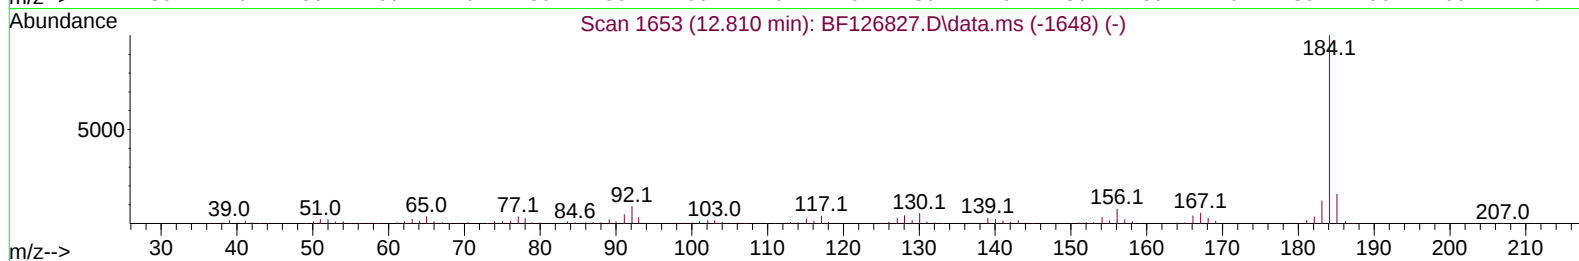
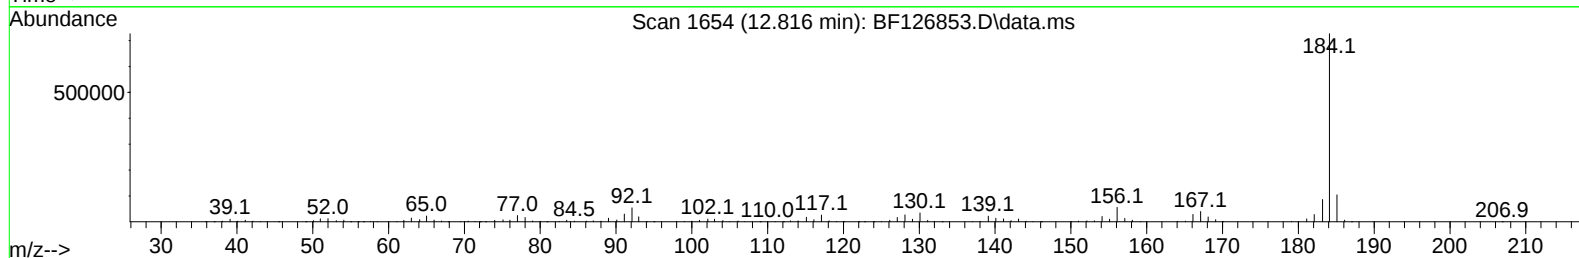


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
Data File : BF126853.D
Acq On : 11 Feb 2022 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 23:17:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

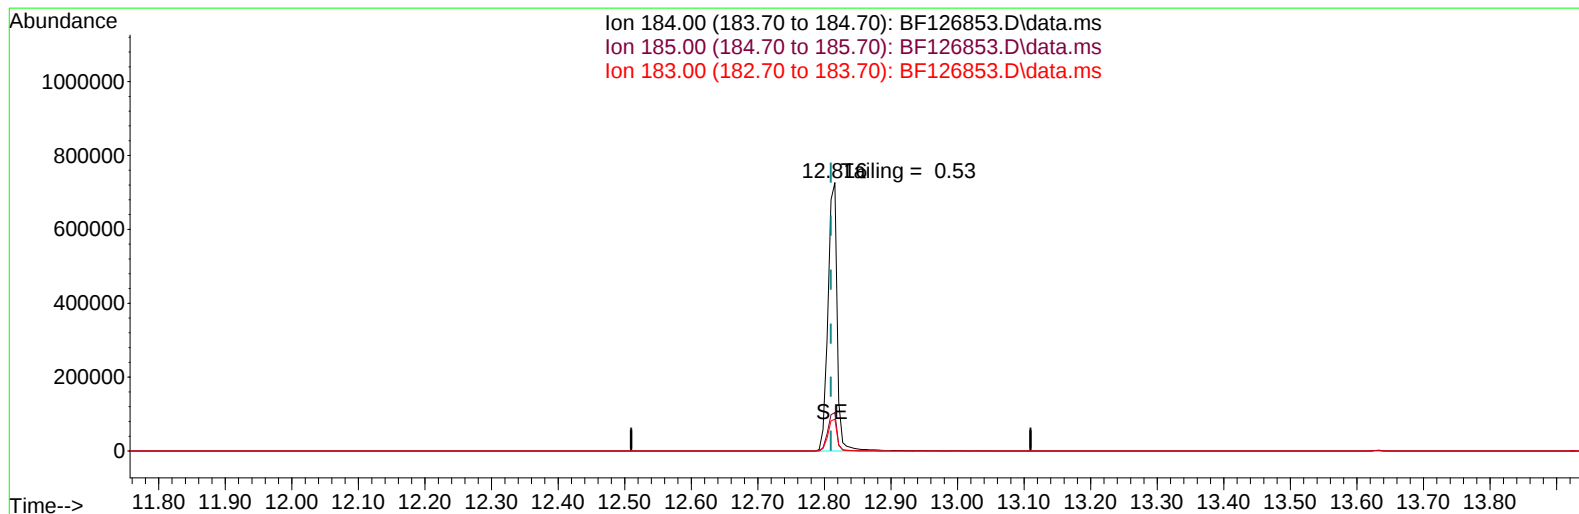

TIC: BF126853.D\data.ms

(77) Benzidine




12.816min (+ 0.006) 0.00 ng

response 701659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.32
183.00	12.00	11.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
 Data File : BF126853.D
 Acq On : 11 Feb 2022 12:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 11 23:17:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 10 00:44:00 2022
 Response via : Initial Calibration

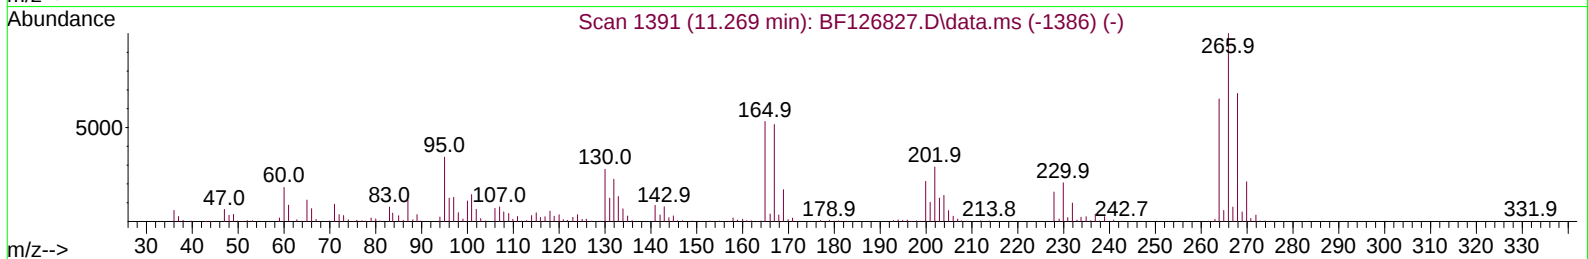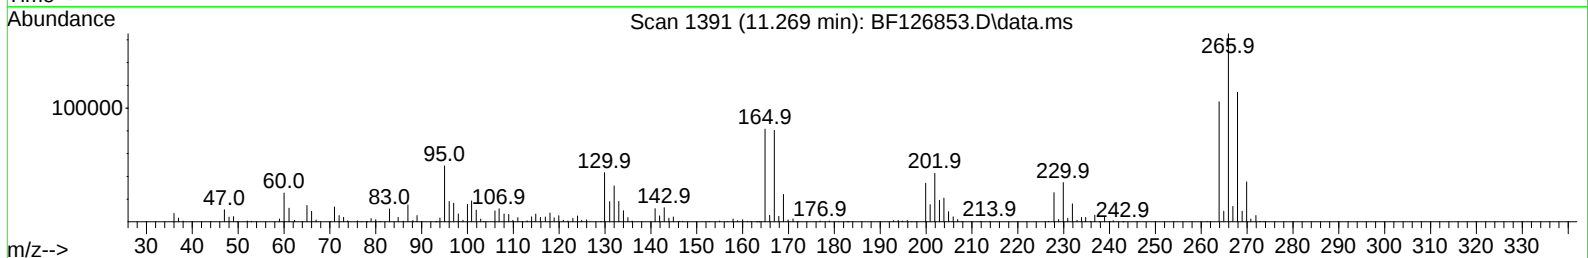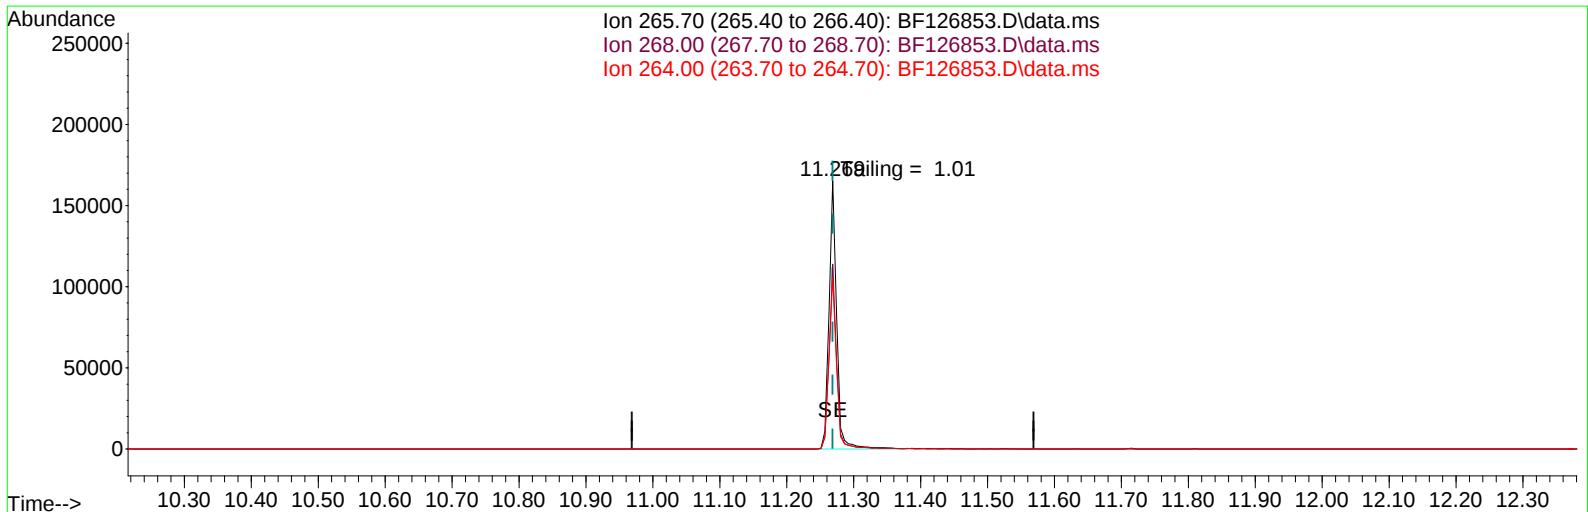

TIC: BF126853.D\data.ms

(70) Pentachlorophenol (C)

11.269min (+ 0.000) 26068.41 ng

response 132102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	68.88
264.00	65.20	63.90
0.00	0.00	0.00