

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
 Data File : BF126863.D
 Acq On : 11 Feb 2022 17:59
 Operator : CG\JU
 Sample : N1489-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.169	485	490	497	rVB	39674	46501	1.86%	0.256%
2	5.551	551	555	558	rBV	2129604	2027819	81.24%	11.153%
3	6.551	720	725	734	rBV	2156124	2190333	87.75%	12.047%
4	6.940	787	791	794	rBV	885572	699569	28.03%	3.848%
5	7.498	882	886	889	rBV	1703256	1470082	58.90%	8.086%
6	8.116	988	991	996	rBV	26958	31301	1.25%	0.172%
7	8.222	1005	1009	1012	rBV	1197771	950494	38.08%	5.228%
8	9.292	1187	1191	1195	rBV	2641754	2420847	96.99%	13.315%
9	9.981	1304	1308	1311	rVB	1192209	1054357	42.24%	5.799%
10	10.292	1356	1361	1364	rBV2	21500	25644	1.03%	0.141%
11	10.386	1371	1377	1382	rVB3	28528	56507	2.26%	0.311%
12	10.769	1438	1442	1445	rBV	1641483	1532771	61.41%	8.430%
13	10.880	1458	1461	1465	rVB3	26926	37321	1.50%	0.205%
14	11.322	1530	1536	1538	rBV3	23839	28324	1.13%	0.156%
15	11.410	1547	1551	1554	rVB3	26871	25550	1.02%	0.141%
16	11.469	1557	1561	1564	rBV	1401323	1140131	45.68%	6.271%
17	11.980	1641	1648	1649	rBV2	22988	28694	1.15%	0.158%
18	12.680	1764	1767	1770	rVB2	36550	32450	1.30%	0.178%
19	12.916	1801	1807	1810	rBV2	29729	36105	1.45%	0.199%
20	13.057	1826	1831	1839	rVB	2656832	2495985	100.00%	13.728%
21	13.945	1979	1982	1985	rBV3	38725	51020	2.04%	0.281%
22	14.110	2006	2010	2014	rBV	766663	698328	27.98%	3.841%
23	14.263	2034	2036	2041	rVB3	27908	30255	1.21%	0.166%
24	14.568	2084	2088	2091	rBV	38322	34686	1.39%	0.191%
25	14.886	2138	2142	2145	rBV	41416	45123	1.81%	0.248%
26	15.168	2186	2190	2194	rBV2	19562	33881	1.36%	0.186%
27	15.239	2198	2202	2207	rVB2	44291	49932	2.00%	0.275%
28	15.621	2261	2267	2284	rBV	526172	712228	28.53%	3.917%
29	16.098	2344	2348	2354	rVB	38553	57983	2.32%	0.319%
30	16.633	2434	2439	2446	rVB2	31504	50113	2.01%	0.276%
31	17.257	2539	2545	2552	rBV2	23191	51453	2.06%	0.283%
32	18.004	2665	2672	2680	rVB5	14323	35614	1.43%	0.196%




Sum of corrected areas: 18181401

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
Data File : BF126863.D
Acq On : 11 Feb 2022 17:59
Operator : CG\JU
Sample : N1489-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

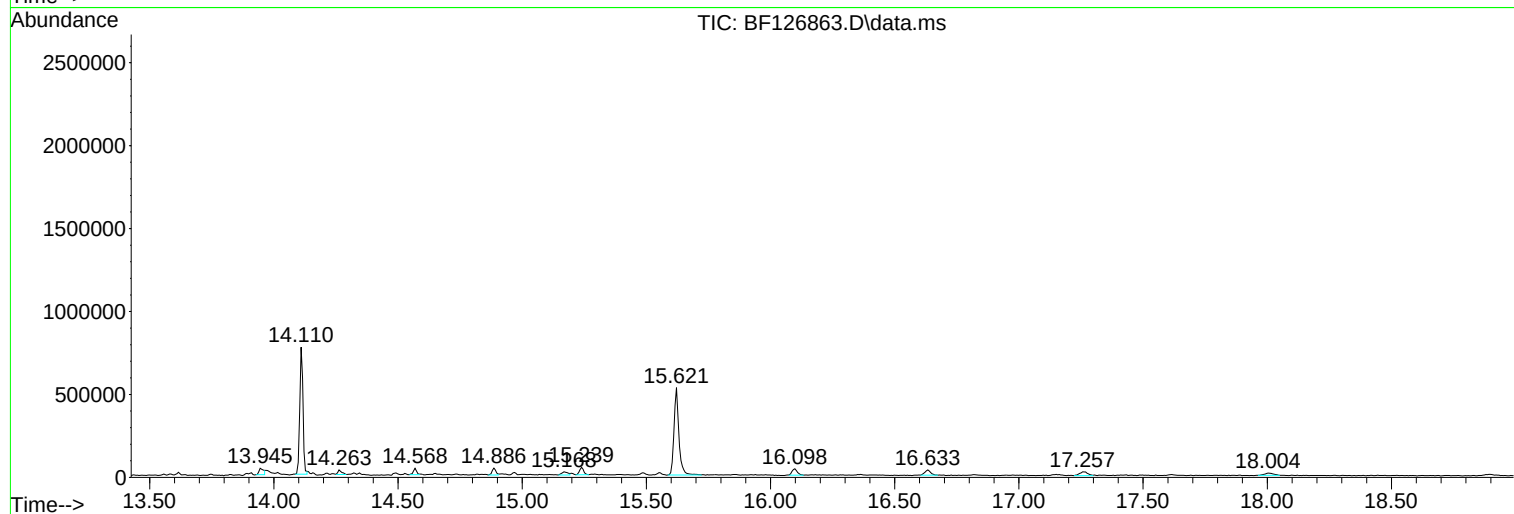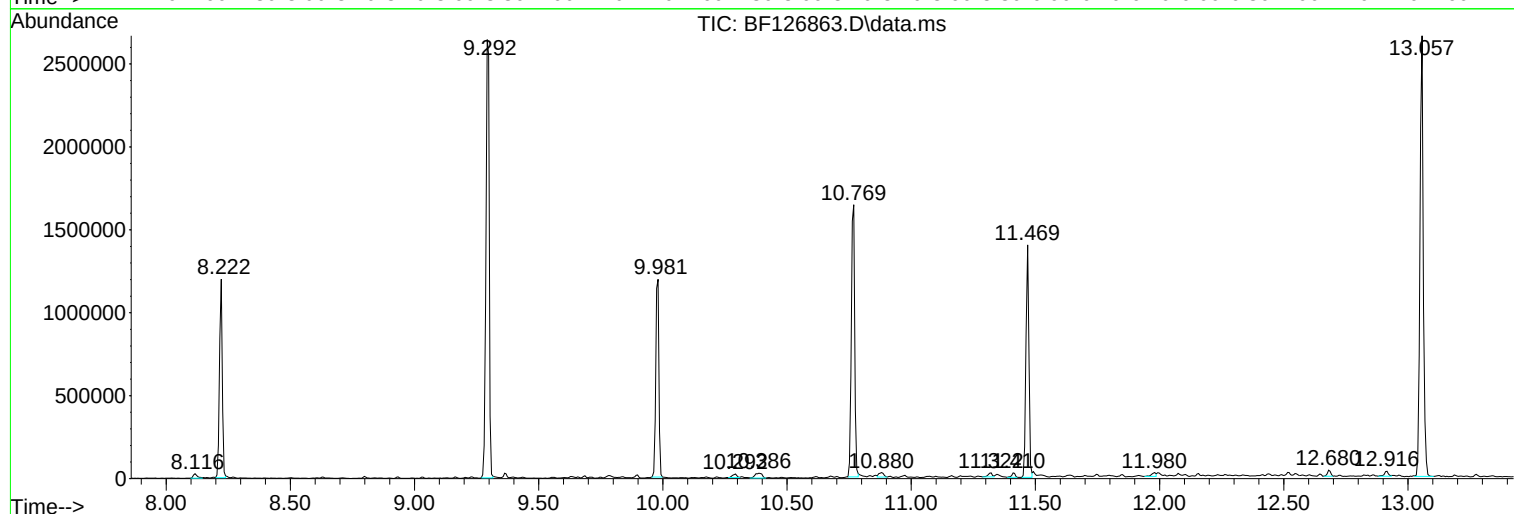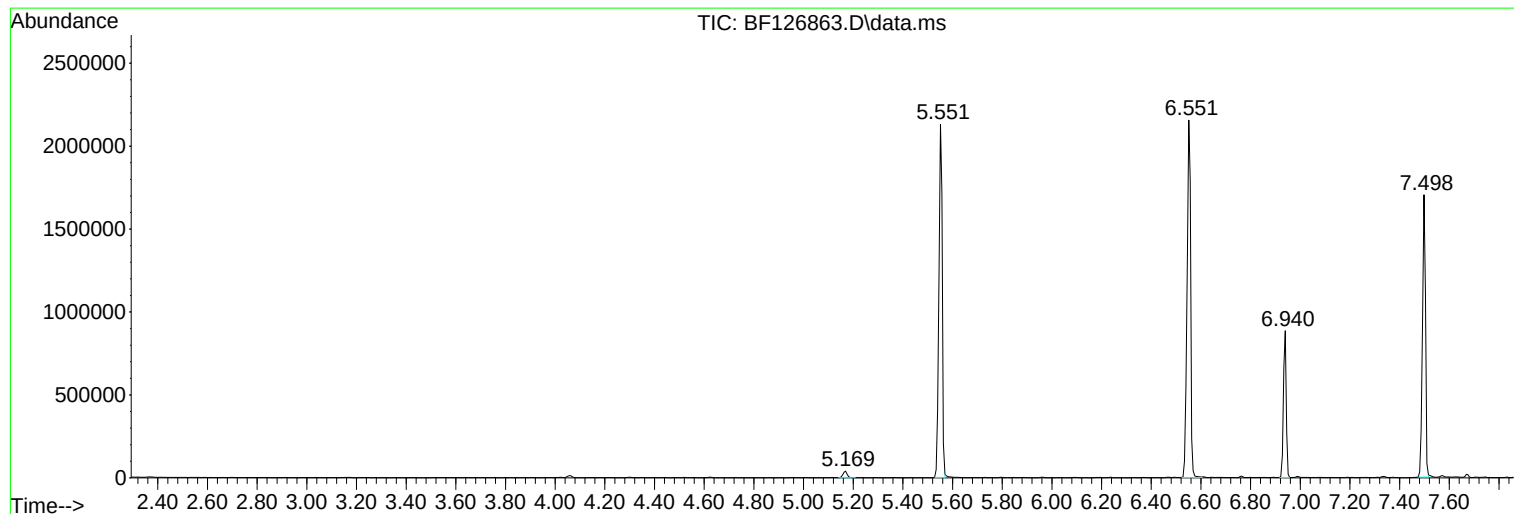

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
Data File : BF126863.D
Acq On : 11 Feb 2022 17:59
Operator : CG\JU
Sample : N1489-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
Data File : BF126863.D
Acq On : 11 Feb 2022 17:59
Operator : CG\JU
Sample : N1489-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------