
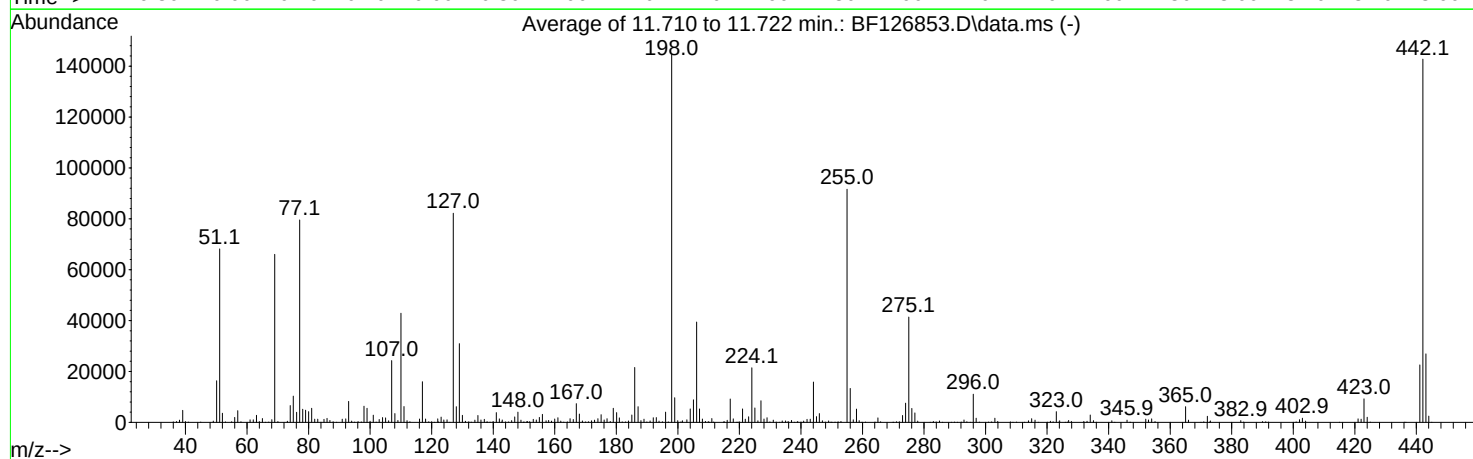


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
 Data File : BF126853.D
 Acq On : 11 Feb 2022 12:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 10 00:44:00 2022

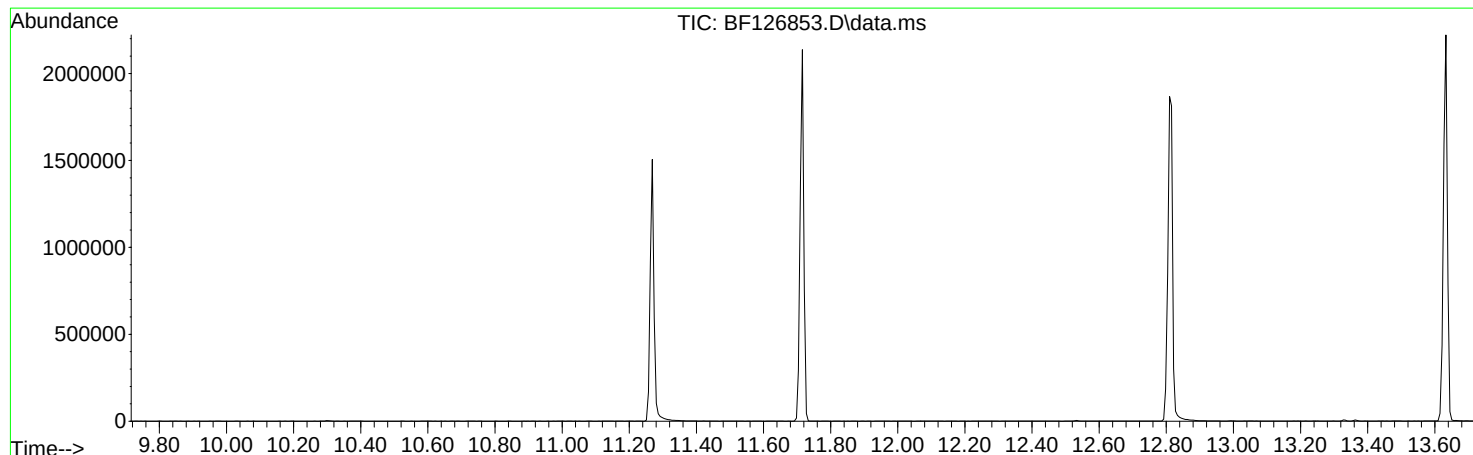

AutoFind: Scans 1466, 1467, 1468; Background Corrected with Scan 1461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	68195	PASS
68	69	0.00	2	1.6	1069	PASS
69	198	0.00	100	45.7	66035	PASS
70	69	0.00	2	0.5	333	PASS
127	198	10	80	56.9	82197	PASS
197	198	0.00	2	0.2	221	PASS
198	198	100	100	100.0	144568	PASS
199	198	5	9	6.7	9689	PASS
275	198	10	60	28.6	41352	PASS
365	198	1	100	4.3	6171	PASS
441	198	0.01	100	15.6	22571	PASS
442	442	50	100	100.0	142752	PASS
443	442	15	24	18.8	26899	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/11/2022	BNA_F	<u>BF126853.D</u>
Compound Name	Response	Retention Time
DDT	323307	13.633
DDD	2532	13.363
DDE	98	12.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2630	325937	0.81

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
Data File : BF126853.D
Acq On : 11 Feb 2022 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 11 23:17:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

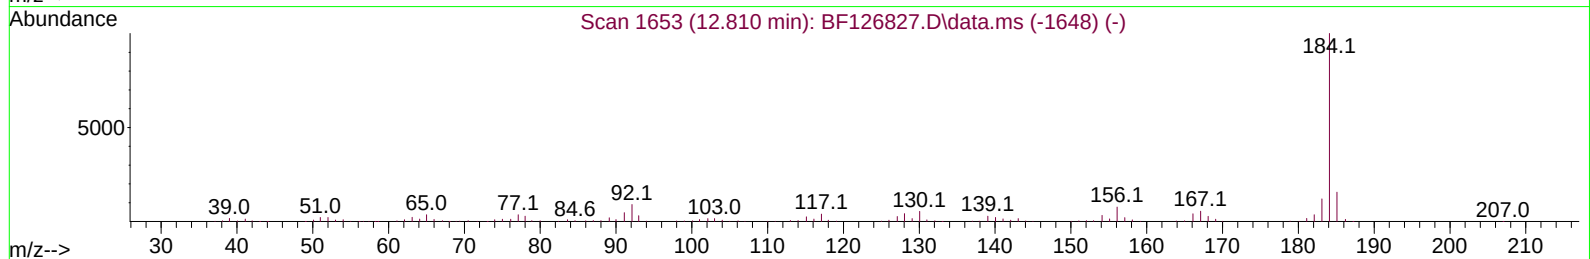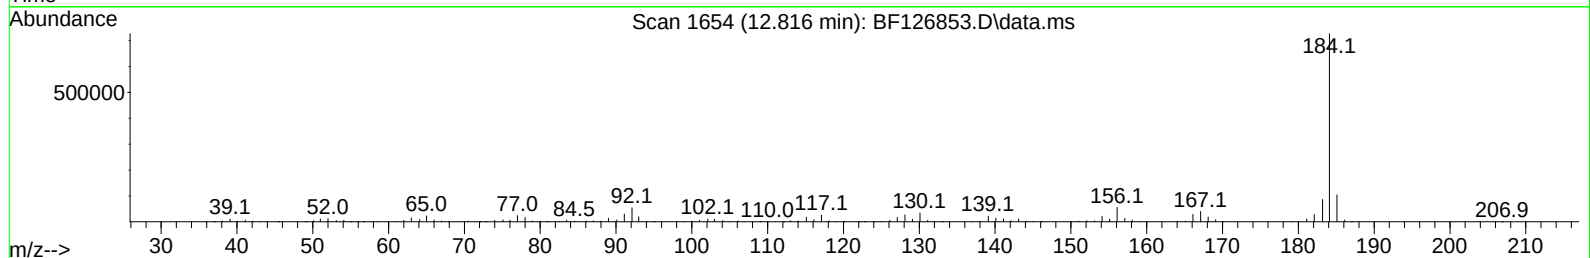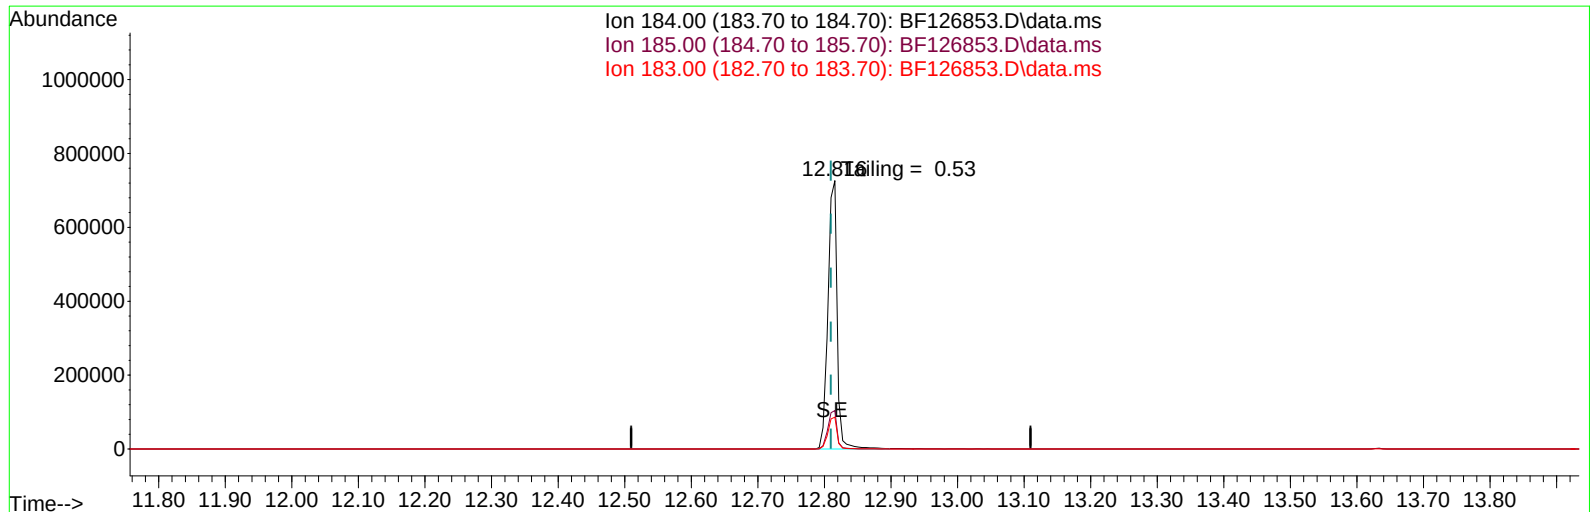

TIC: BF126853.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng




response 701659

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.32
183.00	12.00	11.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021122\
 Data File : BF126853.D
 Acq On : 11 Feb 2022 12:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 11 23:17:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 10 00:44:00 2022
 Response via : Initial Calibration

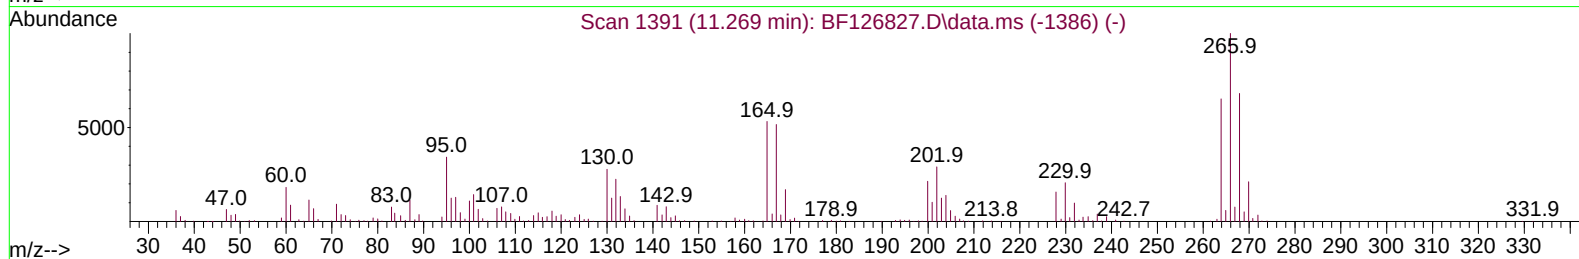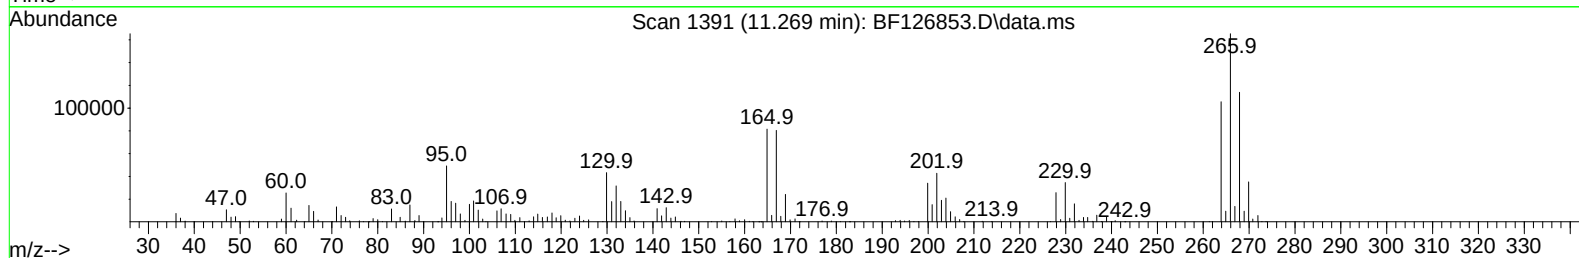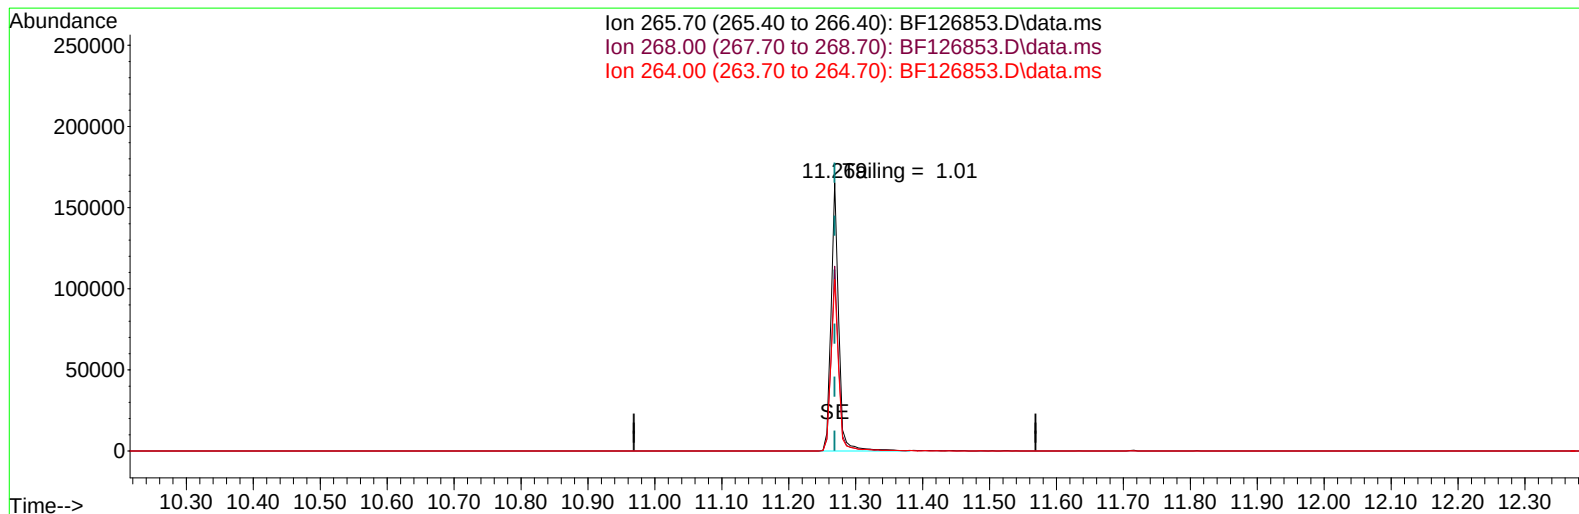

TIC: BF126853.D\data.ms

(70) Pentachlorophenol (C)

11.269min (+ 0.000) 26068.41 ng

response 132102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	68.88
264.00	65.20	63.90
0.00	0.00	0.00