
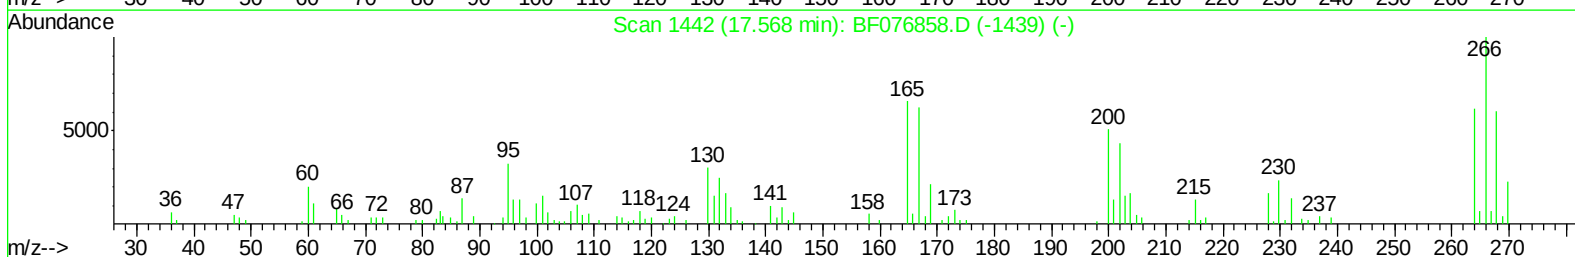
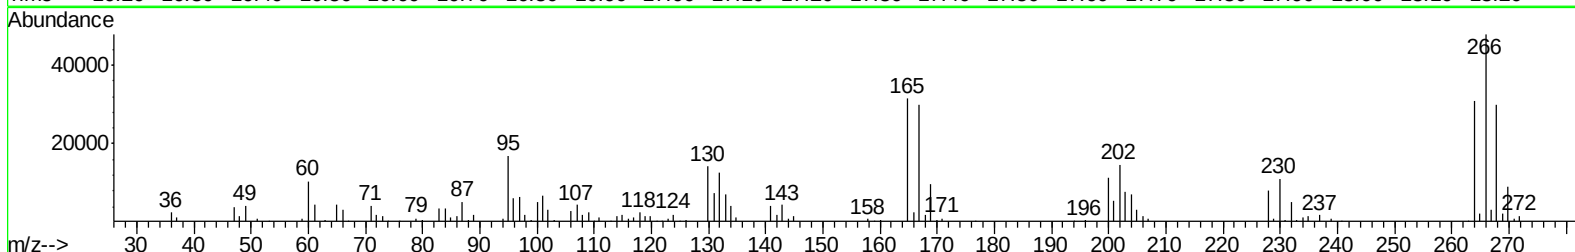


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021215\
Data File : BF077283.D
Acq On : 12 Feb 2015 13:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 07:53:56 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 10 13:30:38 2015
Response via : Initial Calibration

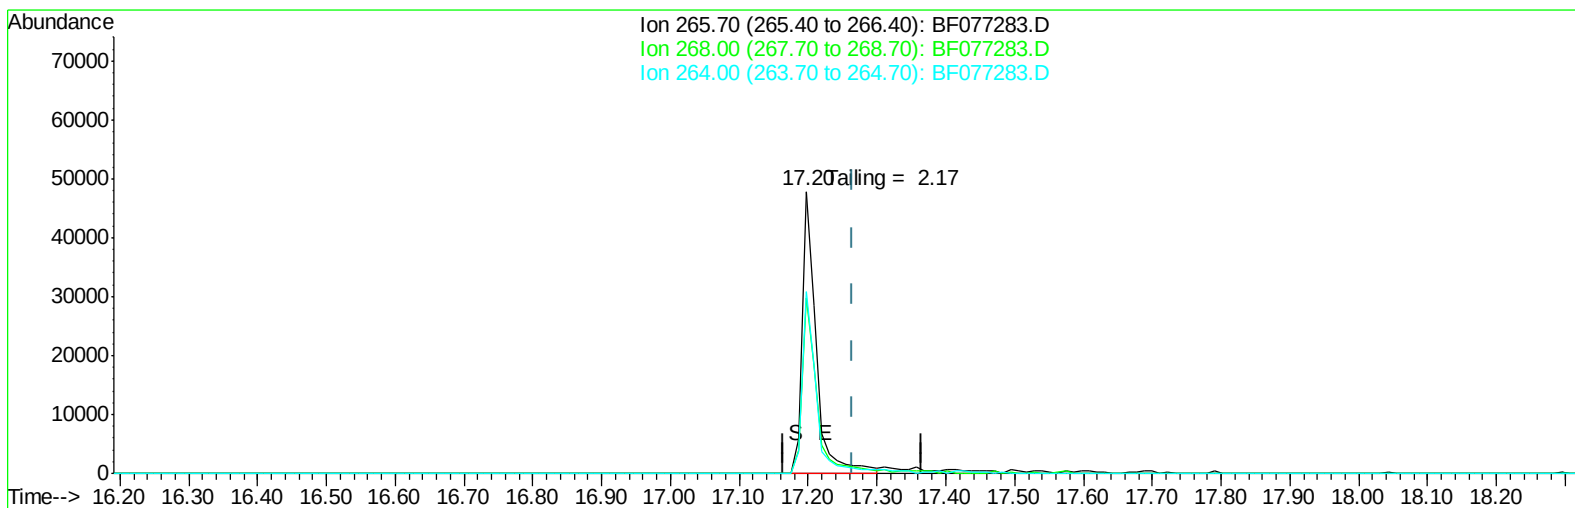

TIC: BF077283.D

(69) Pentachlorophenol (C)




17.197min (-0.069) 0.00ng

response 59524

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.28
264.00	61.90	64.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021215\
 Data File : BF077283.D
 Acq On : 12 Feb 2015 13:32
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 07:53:56 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 10 13:30:38 2015
 Response via : Initial Calibration

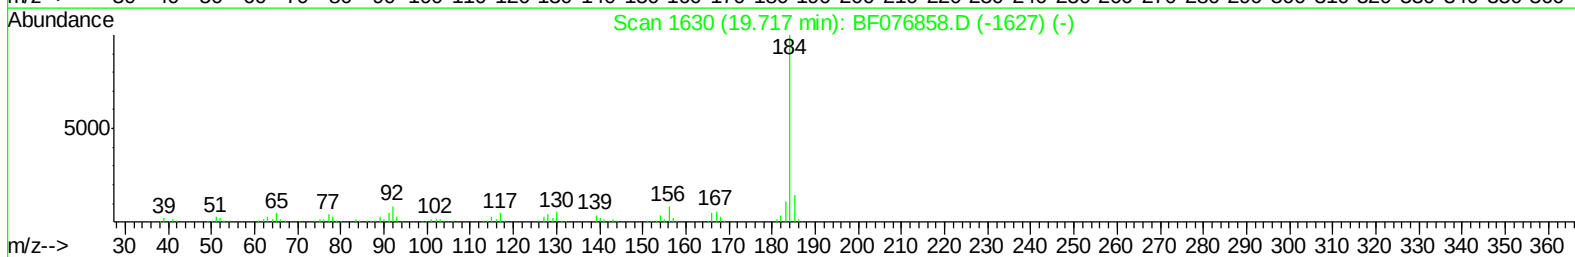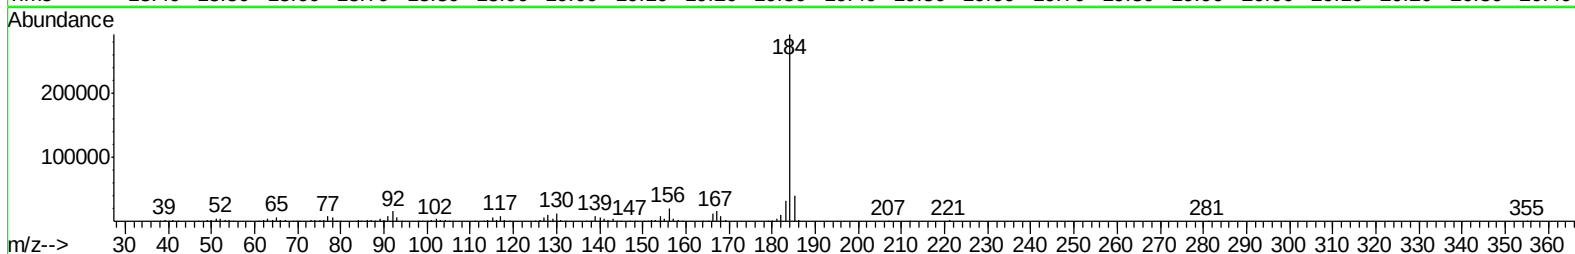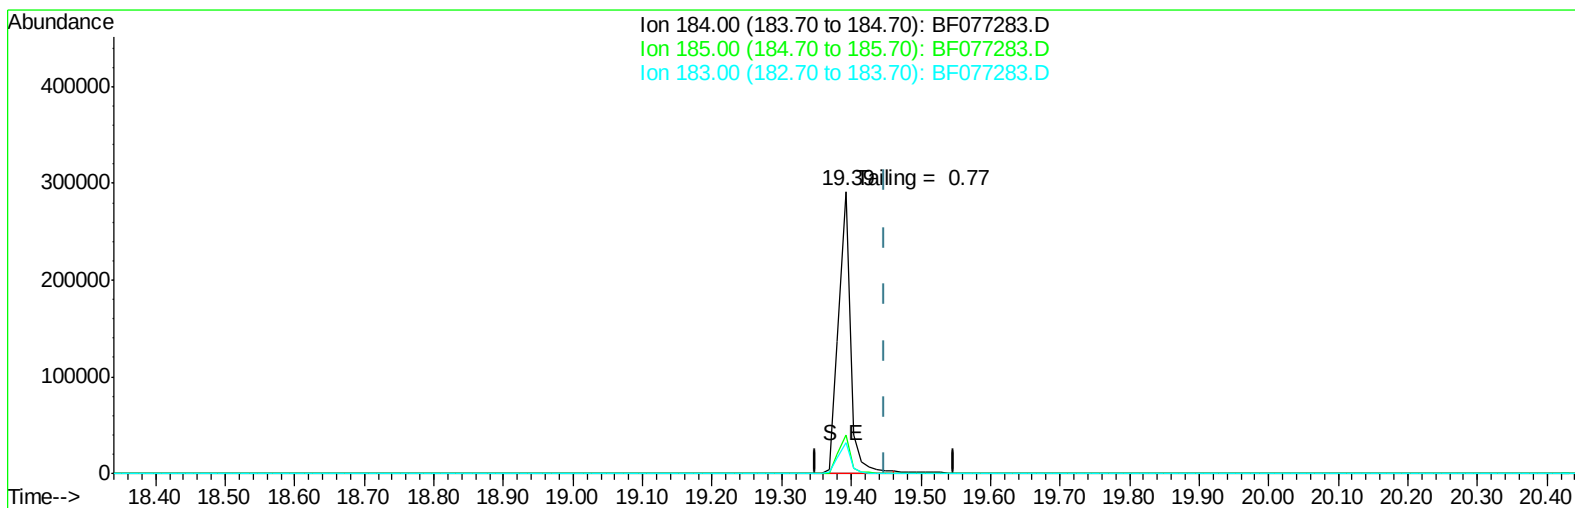

TIC: BF077283.D

(76) Benzidine

19.391min (-0.057) 27390.45ng

response 339195

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	13.80
183.00	11.30	10.93
0.00	0.00	0.00