

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021215\
 Data File : BF077295.D
 Acq On : 12 Feb 2015 21:43
 Operator : TP/IZ
 Sample : G1272-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.104	17	19	23	rBV	11048	19444	1.54%	0.236%
2	1.276	32	34	38	rBV	16836	33980	2.70%	0.413%
3	1.333	38	39	51	rVB	123982	219614	17.44%	2.670%
4	2.487	135	140	144	rVB2	6975	14862	1.18%	0.181%
5	3.493	225	228	241	rBV	89625	262209	20.82%	3.188%
6	4.499	314	316	333	rBV	272338	689267	54.72%	8.380%
7	6.933	526	529	532	rBV	265883	520577	41.33%	6.329%
8	6.990	532	534	543	rVB	505734	914757	72.62%	11.122%
9	7.493	576	578	586	rVB	70533	135833	10.78%	1.651%
10	7.813	603	606	610	rBV	387938	662045	52.56%	8.049%
11	7.870	610	611	615	rVB2	7958	14149	1.12%	0.172%
12	8.808	690	693	703	rBV	328726	528537	41.96%	6.426%
13	10.408	830	833	835	rBV	124020	190268	15.11%	2.313%
14	10.454	835	837	843	rVB	43552	79600	6.32%	0.968%
15	12.122	981	983	987	rBB	10325	17840	1.42%	0.217%
16	13.060	1062	1065	1069	rBV	616620	1073016	85.19%	13.046%
17	14.523	1190	1193	1198	rBB	127845	211101	16.76%	2.567%
18	16.077	1327	1329	1332	rBB	15437	23543	1.87%	0.286%
19	16.294	1345	1348	1357	rBB	477956	665557	52.84%	8.092%
20	17.437	1445	1448	1451	rBV	162129	227131	18.03%	2.761%
21	19.689	1643	1645	1648	rBV	885526	1259585	100.00%	15.314%
22	20.946	1753	1755	1758	rBV	214341	242096	19.22%	2.943%
23	22.581	1895	1898	1902	rBV	157925	219997	17.47%	2.675%


Sum of corrected areas: 8225008

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021215\
Data File : BF077295.D
Acq On : 12 Feb 2015 21:43
Operator : TP/IZ
Sample : G1272-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

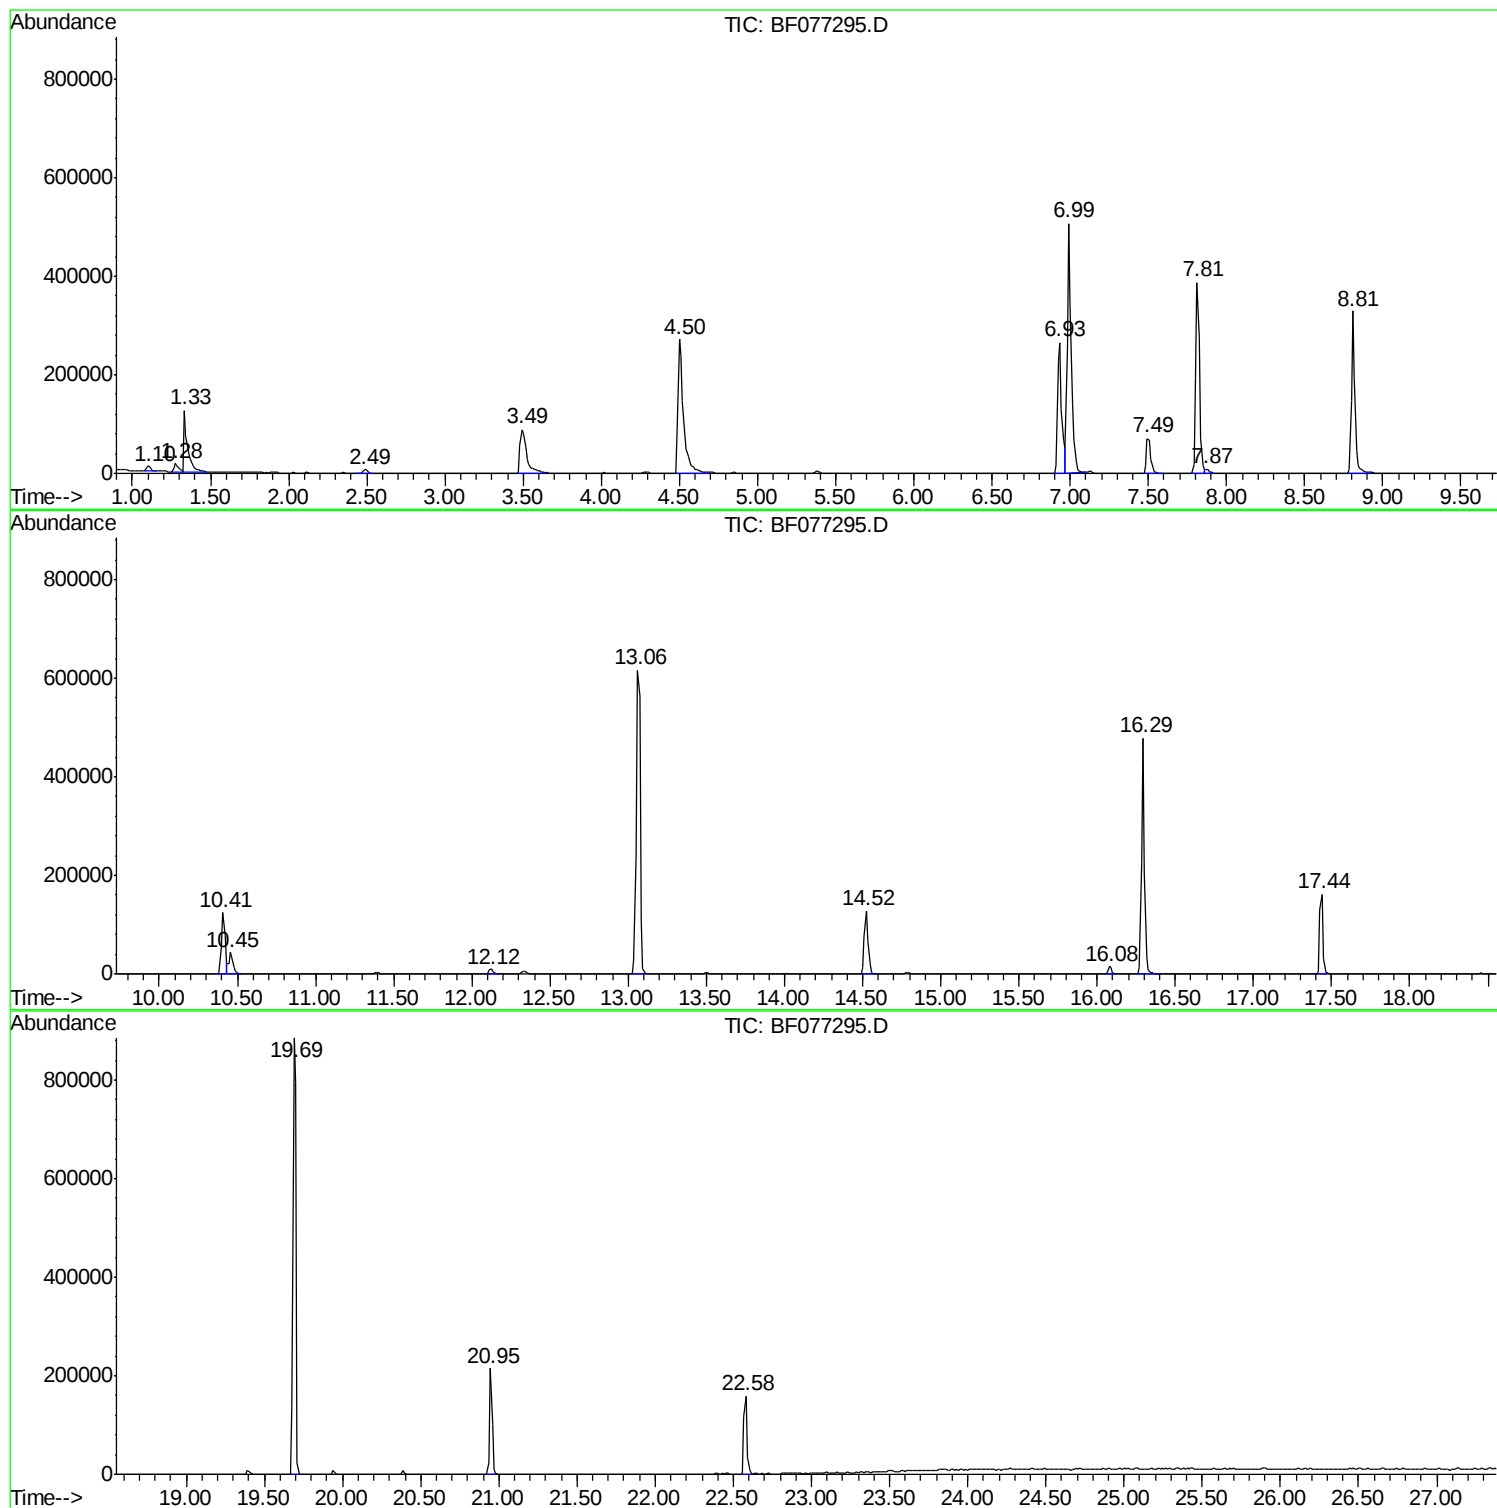

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF021215\
Data_File : BF077295.D
Acq_On : 12_Feb_2015 21:433
Operator : TP/IZZ
Sample : G1272-022
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
WC-1

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
