

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF021215\  
 Data File : BF077298.D  
 Acq On : 12 Feb 2015 23:27  
 Operator : TP/IZ  
 Sample : G1253-05  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 WC-SLDG-WT-70

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF021215.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.276       | 32            | 34          | 38           | rBV      | 10957          | 19179         | 1.75%           | 0.250%        |
| 2         | 1.333       | 38            | 39          | 52           | rVB      | 41480          | 79731         | 7.29%           | 1.040%        |
| 3         | 3.481       | 225           | 227         | 247          | rBV      | 74743          | 230689        | 21.09%          | 3.010%        |
| 4         | 4.499       | 313           | 316         | 332          | rBV      | 318518         | 749690        | 68.55%          | 9.782%        |
| 5         | 6.922       | 526           | 528         | 531          | rBV      | 405600         | 654141        | 59.82%          | 8.535%        |
| 6         | 6.990       | 531           | 534         | 545          | rVB      | 469304         | 898546        | 82.17%          | 11.724%       |
| 7         | 7.493       | 576           | 578         | 586          | rBB      | 84128          | 149768        | 13.70%          | 1.954%        |
| 8         | 7.813       | 603           | 606         | 615          | rBV      | 377037         | 613869        | 56.13%          | 8.010%        |
| 9         | 8.808       | 690           | 693         | 705          | rBV      | 294035         | 477133        | 43.63%          | 6.226%        |
| 10        | 10.408      | 830           | 833         | 843          | rBV      | 121719         | 202975        | 18.56%          | 2.648%        |
| 11        | 13.060      | 1062          | 1065        | 1069         | rBV      | 574874         | 965591        | 88.30%          | 12.599%       |
| 12        | 14.523      | 1190          | 1193        | 1200         | rBB2     | 138031         | 232489        | 21.26%          | 3.033%        |
| 13        | 16.294      | 1345          | 1348        | 1360         | rBB      | 387178         | 550739        | 50.36%          | 7.186%        |
| 14        | 17.437      | 1445          | 1448        | 1451         | rBV      | 170963         | 244210        | 22.33%          | 3.186%        |
| 15        | 19.689      | 1643          | 1645        | 1648         | rBV      | 867712         | 1093576       | 100.00%         | 14.269%       |
| 16        | 20.946      | 1753          | 1755        | 1758         | rBV      | 188070         | 252788        | 23.12%          | 3.298%        |
| 17        | 22.581      | 1895          | 1898        | 1904         | rBV      | 188716         | 236454        | 21.62%          | 3.085%        |
| 18        | 25.907      | 2185          | 2189        | 2194         | rBV5     | 3208           | 12588         | 1.15%           | 0.164%        |


Sum of corrected areas: 7664156

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF021215\  
Data File : BF077298.D  
Acq On : 12 Feb 2015 23:27  
Operator : TP/IZ  
Sample : G1253-05  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
WC-SLDG-WT-70

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF021215.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

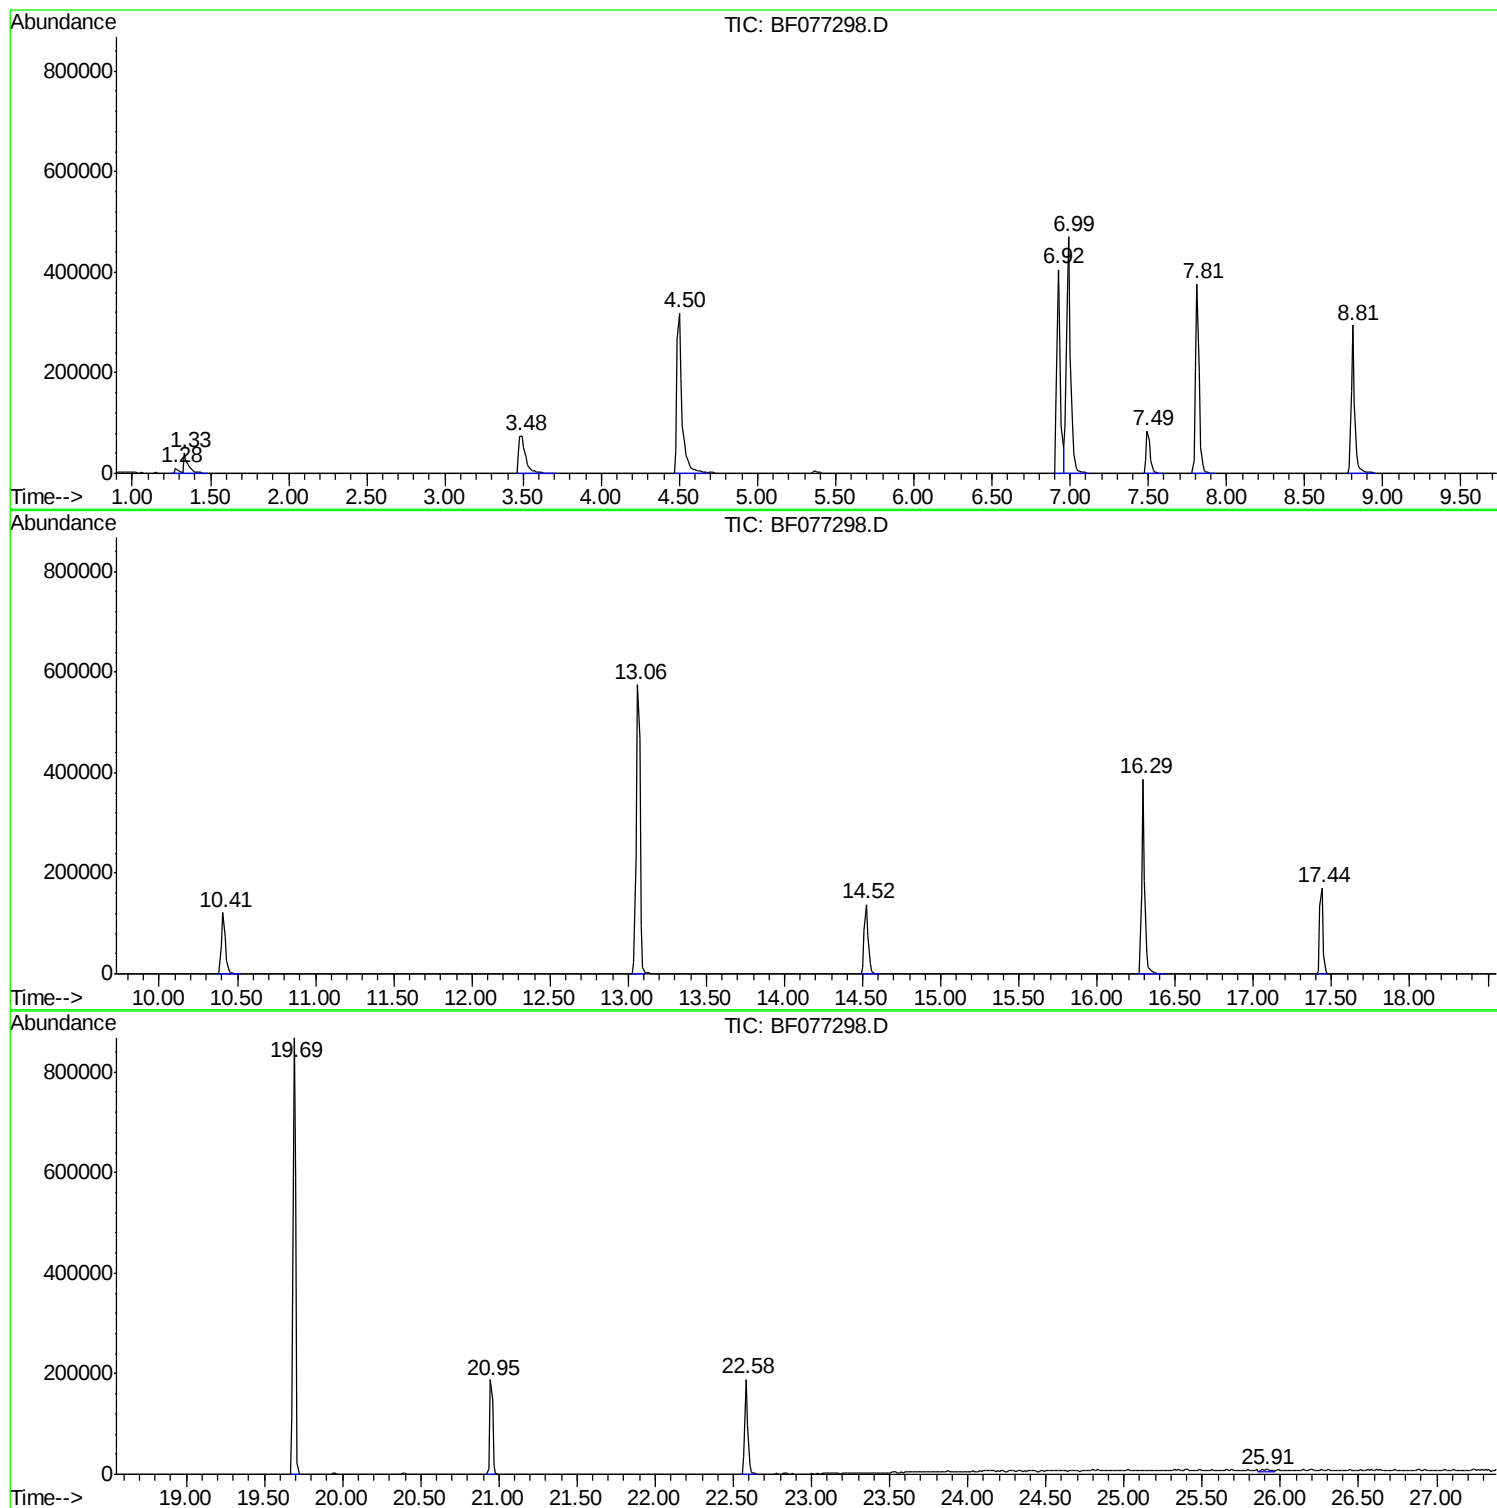

Data\_Path : Z:\HPCHEM1\BNA\_F\DATA\BF021215\  
Data\_File : BF077298.D  
Acq\_On : 12\_Feb\_2015\_ 23:277  
Operator : TP/IZZ  
Sample : G1253-055  
Misc :  
ALS\_Vial : 17 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
WC-SLDG-WT-70

Quant\_Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF021215.MM  
Quant\_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC\_Library : C:\DATABASE\NIST02.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       | #        | RT Resp Conc            |

No Library Search Compounds Detected

\*\*\*\*\*