

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021215\
 Data File : BF077301.D
 Acq On : 13 Feb 2015 1:11
 Operator : TP/IZ
 Sample : G1270-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WC-060-21015

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.333	38	39	49	rVB	29041	53375	1.28%	0.180%
2	1.767	74	77	86	rVB	113862	178070	4.26%	0.601%
3	2.361	126	129	139	rBV	54872	122546	2.93%	0.414%
4	3.493	225	228	243	rBV	82660	236394	5.65%	0.798%
5	4.499	314	316	330	rBV	287923	746845	17.86%	2.521%
6	6.979	526	533	534	rBV	679785	1481888	35.44%	5.002%
7	7.150	542	548	551	rVB	1553787	4181588	100.00%	14.115%
8	7.390	563	569	572	rBV	861375	1621319	38.77%	5.473%
9	7.505	575	579	585	rVV	236670	426824	10.21%	1.441%
10	7.813	601	606	610	rBV2	428753	977886	23.39%	3.301%
11	7.870	610	611	615	rVB2	28967	46666	1.12%	0.158%
12	7.973	618	620	627	rBV	32139	76972	1.84%	0.260%
13	8.579	670	673	675	rBV	27179	42332	1.01%	0.143%
14	8.808	690	693	701	rVB	348567	601360	14.38%	2.030%
15	9.333	703	739	741	rBV2	201797	2155362	51.54%	7.275%
16	9.413	741	746	748	rBV2	69557	232521	5.56%	0.785%
17	9.722	761	773	777	rBV	125352	580926	13.89%	1.961%
18	9.928	777	791	794	rBV	452004	1511582	36.15%	5.102%
19	10.122	804	808	810	rBV	152256	448801	10.73%	1.515%
20	10.236	810	818	819	rVV3	278357	1285932	30.75%	4.341%
21	10.282	819	822	823	rVV2	200659	393056	9.40%	1.327%
22	10.374	823	830	831	rVV2	194518	648137	15.50%	2.188%
23	10.408	831	833	836	rVV	341258	498348	11.92%	1.682%
24	10.454	836	837	841	rVB	77165	96023	2.30%	0.324%
25	10.534	841	844	846	rBV2	33108	57936	1.39%	0.196%
26	10.716	854	860	863	rBV	51638	109509	2.62%	0.370%
27	10.796	863	867	871	rVB	72408	155761	3.72%	0.526%
28	11.185	897	901	905	rBV2	29041	89209	2.13%	0.301%
29	11.334	905	914	916	rBV2	52975	205318	4.91%	0.693%
30	11.471	923	926	928	rBV	246417	424140	10.14%	1.432%
31	11.539	928	932	935	rBV	54434	102729	2.46%	0.347%
32	11.722	938	948	950	rBV4	80547	352621	8.43%	1.190%
33	11.951	953	968	971	rBV5	112445	857334	20.50%	2.894%
34	12.145	980	985	987	rBV3	177169	458814	10.97%	1.549%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021215\
Data File : BF077301.D
Acq On : 13 Feb 2015 1:11
Operator : TP/IZ
Sample : G1270-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WC-060-21015

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.339	1000	1002	1005	rVB3	291477	536027	12.82%	1.809%
36	12.419	1005	1009	1010	rBV	101370	207150	4.95%	0.699%
37	12.454	1010	1012	1013	rBV	48974	64843	1.55%	0.219%
38	12.499	1013	1016	1018	rBV2	53188	140693	3.36%	0.475%
39	12.625	1024	1027	1028	rBV2	38567	78663	1.88%	0.266%
40	12.728	1028	1036	1040	rVB3	147956	698279	16.70%	2.357%
41	12.865	1046	1048	1051	rVB2	25235	43911	1.05%	0.148%
42	13.071	1062	1066	1069	rVB	633852	1120887	26.81%	3.784%
43	13.997	1144	1147	1151	rVB	60632	107501	2.57%	0.363%
44	14.523	1189	1193	1200	rVB2	360981	617179	14.76%	2.083%
45	16.294	1345	1348	1356	rVB	493733	707960	16.93%	2.390%
46	16.431	1356	1360	1363	rBV	45476	74059	1.77%	0.250%
47	17.437	1445	1448	1451	rBV	488742	649168	15.52%	2.191%
48	18.454	1535	1537	1541	rBV	111524	136903	3.27%	0.462%
49	19.597	1635	1637	1643	rVB	85408	108768	2.60%	0.367%
50	19.700	1643	1646	1648	rBV	887363	1290535	30.86%	4.356%
51	20.363	1701	1704	1706	rBV	178388	195696	4.68%	0.661%
52	20.843	1743	1746	1748	rBV	40653	44772	1.07%	0.151%
53	20.946	1753	1755	1758	rBV	487060	701289	16.77%	2.367%
54	22.592	1896	1899	1902	rBV	527948	642537	15.37%	2.169%


Sum of corrected areas: 29624944

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021215\
Data File : BF077301.D
Acq On : 13 Feb 2015 1:11
Operator : TP/IZ
Sample : G1270-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WC-060-21015

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

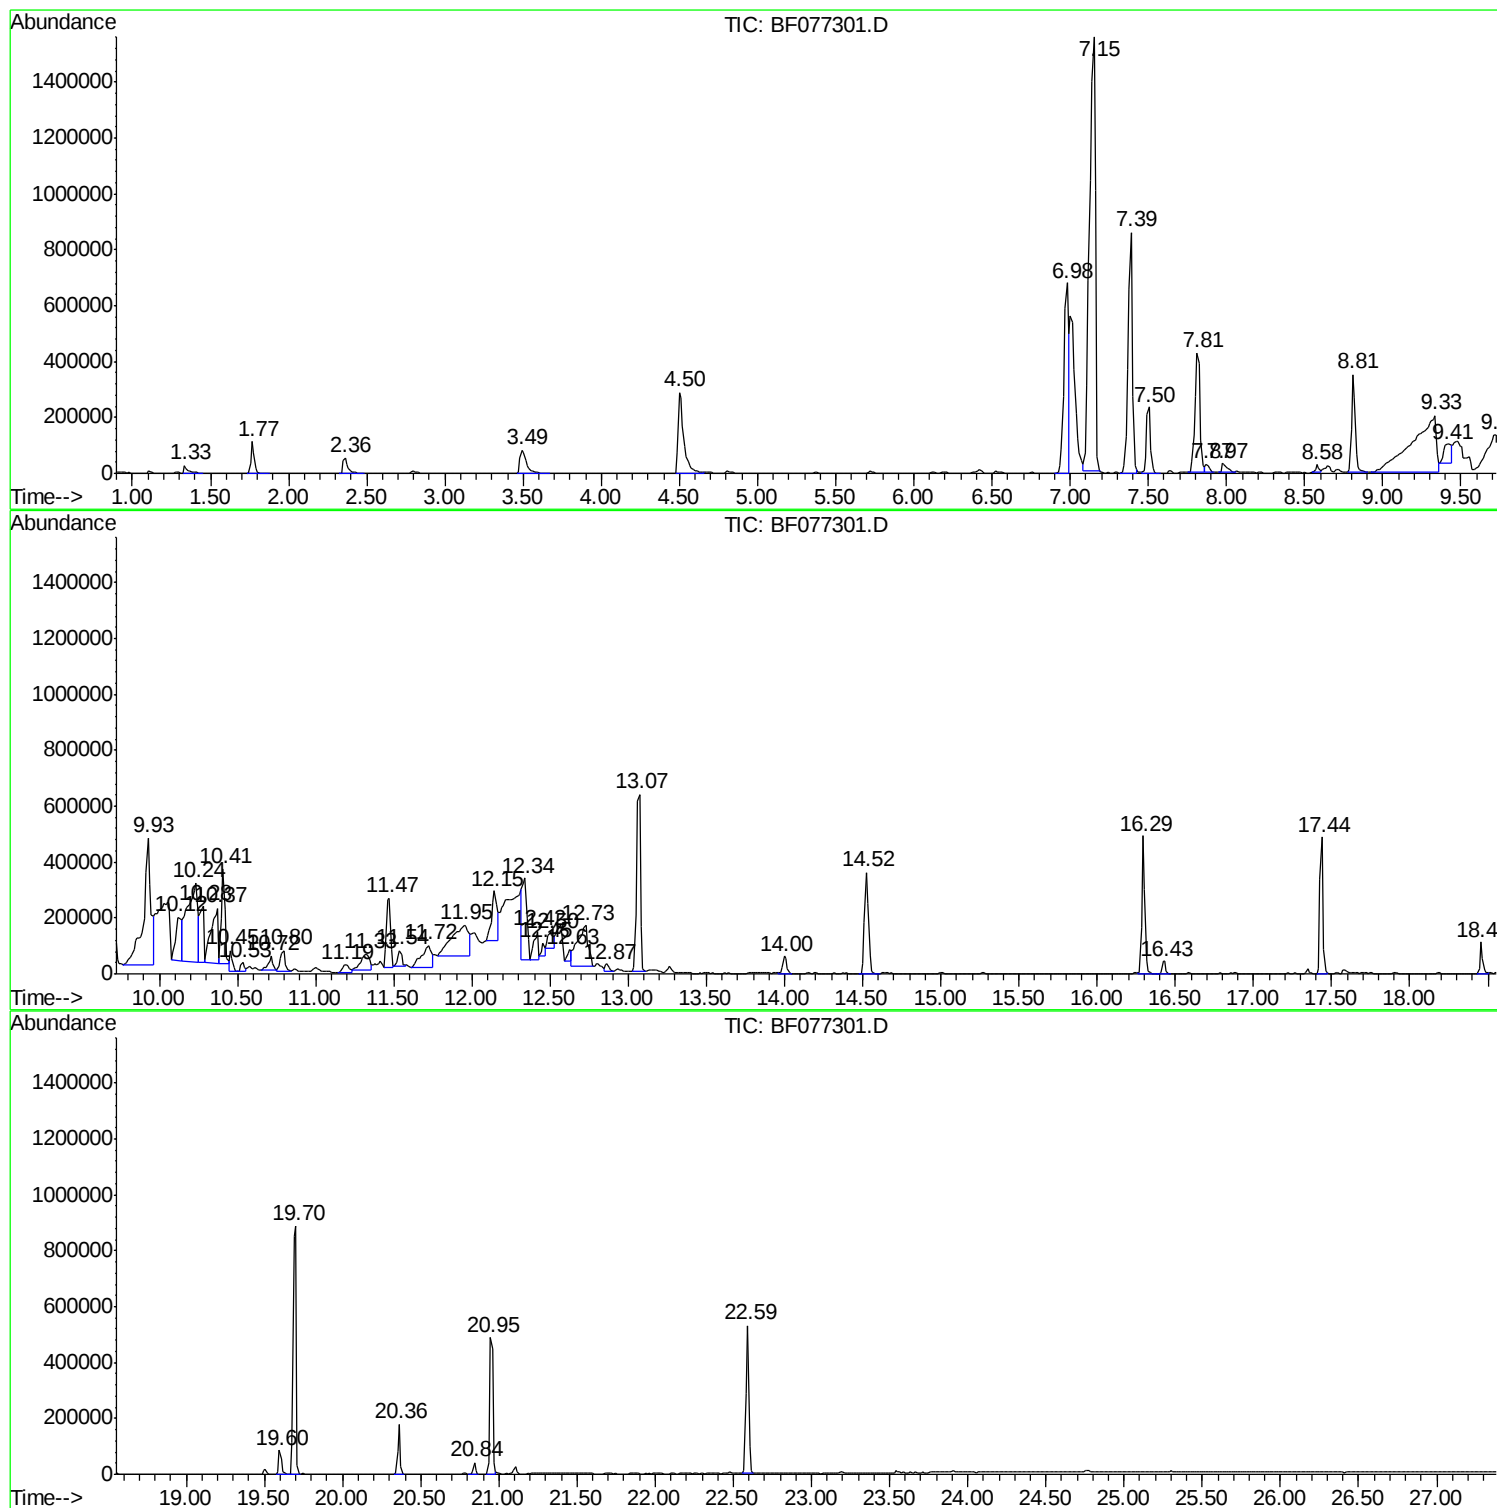

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF021215\
Data_File : BF077301.D
Acq_On : 13_Feb_2015 1:111
Operator : TP/IZZ
Sample : G1270-022
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
DCW-WC-060-21015

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021215.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
